

# NT

*digital implant technology*



**PRODUCT CATALOGUE 2017-1**

# CONTACT INFORMATION

## TECHNICAL SUPPORT

Please contact your local dealer or nt-trading directly.

Email: [support@nt-trading.com](mailto:support@nt-trading.com)  
Phone: +49 (0)721 / 91 54 71-60

## ORDER

We have distributors in more than 35 countries.

Please contact your local dealer or nt-trading directly.

Email: [info@nt-trading.com](mailto:info@nt-trading.com)  
Phone: +49 (0)721 / 91 54 71-60

# SAFETY - INNOVATION - RELIABILITY

*MORE THAN ABUTMENT SOLUTIONS – EXPERIENCE THE QUALITY*

Worldwide confidence users in more than over 40 countries rely to the nt-trading abutment solutions. In the year of 2015 hundreds of thousand prosthetic implant treatments used nt-trading Abutments, which is now documentable in the nt-trading implant pass.

With the nt-trading implant pass, the patient get all necessary information. It conduces to collect the important information of the implantology treatments patient-customized documentation.

Regular control examination in the dentist praxis are important, to recognize possible issues early on. Ensure for the documentation of the control examination, that in the designated columns of the nt-trading implant pass, the date of the control examination and seal of the dentist practice deposited there.

*FOR MORE INFORMATION PLEASE CONTACT ABOVE.*



# MORE THAN ABUTMENTS

**NT** stands for unceasing technology innovation to improve security and quality for medical devices - **MADE IN GERMANY** ///



## PATENTS:

### 3D-Guide & Scan Body:

- Patent in USA (5000.P0271US)
- Patents in Germany, Europe, Japan

### Preform Blank Holder:

- European Patent (EP2013/054986)

### Implant Analog for Digital Models (DIM Analog)

- PCT/EP pending

### Implant Abutment 2CONnect

- Patent in Europe

### Transfer Device / Validation Check

- PCT/EP pending

## TM

## TRADEMARKS:

### 3D-Guide & Scan Body®:

- Registered Trademark in USA, Europe

### Implant Abutment 2CONnect®

- EU Trademark No. 009730532, 15/07/2011
- US Trademark No. 79/100903,
- Japan Trademark No. 100-8915



### OptiScan®

- EU Trademark. 009792821, 18/08/2011

### nt-Preform®

- EU Trademark No. 011265188

## STRENGTH AND FATIGUE TEST ACCORDING TO ISO 14801



## NT-TRADING MEETS THE REQUIREMENTS OF:

- ISO 13485 : 2012 and EU Directive 93/42/EEC
- GOST-R (Russia)
- CMDCAS GD210 (Canada)
- QSR 21 CFR 820 (United States)
- JGMP/PAL (Japan)
- CFDA-MDR (China)



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 🇺🇸

# NT-TRADING EMPIRICAL

## SETTING NEW STANDARDS!

nt-trading GmbH & Co. KG is a leading, global premium manufacturer of high-end dental medical products and a pioneer in the development of digital application products for dental implantology. Through pioneering innovations, technologically advanced products, excellent manufacturing processes and safe application solutions, nt-trading supports its customers in the long term and thus ensures decisive competitive advantages. We consider ourselves to be a forward-thinking company that identifies future developments and implements innovative products. This means that we can support the work of our customers in a particularly targeted manner. The key to our success is our investment in our customers' success. We offer an innovative range of products for creative people without the constraints of a system.

## SUCCESS THROUGH QUALITY

Our quality standards are reflected in a promise to all those who come into contact with us and our products. By this, we mean reliability, respect and compliance with the highest standards – for our products, our services and our actions. We work in many ways to meet these standards: We are certified in accordance with EN ISO 13485, Directive 93/42/EEC and CMDCAS GD210 (Canada). As a global exporter, we meet the requirements of QSR 21 CFR 820 (USA), GOST-R (Russia) and GMP/MHLW (Japan). In over 40 countries around the world, nt-trading products are used to treat patients for whom we produced hundreds of thousands of medical products in 2015.

## NT-TRADING GMBH & CO. KG IS MORE THAN A MANUFACTURER. NT-TRADING GMBH & CO. KG IMPLEMENTS SYSTEM SOLUTIONS.

At our production facility in Karlsruhe, we carry out both product development and manufacturing in order to ensure the long-term quality standards



required for the demanding nt-trading products which are oriented to the needs of our customers all over the world. Our products are carefully manufactured using the latest sophisticated production processes. This is how we ensure a high level of vertical integration – a requirement for producing the best possible manufacturing and processing quality.

All processes, from development through to delivery, are located under one roof. We are therefore clearly committed to using Germany as the location from which we will meet the extensive quality requirements of the international dental medical technology sector.

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# NT-TRADING EMPIRICAL




## DYNAMIC PERSPECTIVES

Dirk Jahn and Andreas Schütt, as managing directors, have defined the nt-trading philosophy as follows:

„Innovative – top quality – customer-oriented“. Together with their employees, this philosophy is continuously bringing a new dynamism. Think globally, act locally – but predominantly, acting with a sense of responsibility and with mutual respect are the common values determining our day-to-day conduct.

From the outset, we have placed great importance on ongoing research and development work in cooperation with well-known university hospitals and institutes. This ensures that we can conti-



nuously develop the range of products for dental CAD/CAM implantology. We are thereby laying the foundation for ensuring the highest standards for our users and their patients. Alongside product development, Dirk Jahn – as a member of the guideline committee of the Association of German Engineers VDI 5705 „Digital process chains in industrial medical technology“ – is heavily involved in the development of national standards.

The unique products from nt-trading either have a global patent or are patent pending. This allows us to secure the potential for future further development of our products and application processes. Based on our core skills and the „Made and Engineered in Germany“ expertise associated with this, we are specifically focusing on promoting and strengthening our partnerships with global users.

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# NT-TRADING EMPIRIE

## MASSTÄBE SETZEN!

Die nt-trading GmbH & Co. KG ist ein führender, global agierender Premiumhersteller für dentale High-End Medizinprodukte und ein Pionier in der Entwicklung digitaler Applikationsprodukte für die dentale Implantologie. Durch wegweisende Innovationen, technisch führende Produkte, exzellente Fertigungsverfahren und sichere Anwendungslösungen unterstützt nt-trading seine Kunden nachhaltig und sichert somit entscheidende Wettbewerbsvorteile. Wir sehen uns dabei in der Rolle eines Vordenkers, der zukünftige Entwicklungen erkennt und in innovative Produkte umsetzt. Dadurch können wir unsere Kunden besonders zielgerichtet in ihrer Arbeit unterstützen.

## ERFOLG DURCH QUALITÄT

Unser Qualitätsanspruch ist ein Versprechen an alle, die mit uns und unseren Produkten in Kontakt treten. Darunter verstehen wir Zuverlässigkeit, Wertschätzung und die Einhaltung höchster Standards – für unsere Produkte, unsere Leistungen und unser Handeln. Um diesem Anspruch gerecht zu werden, tun wir einiges: Wir sind nach EN ISO 13485, der Richtlinie 93/42/EWG und CMDCAS GD210 (Kanada) zertifiziert. Als weltweiter Exporteur erfüllen wir die Anforderungen der QSR 21 CFR 820 (USA), GOST-R (Russland) und GMP/MHLW (Japan). In über 40 Ländern weltweit werden Patienten mit nt-trading Produkten behandelt, für die wir im Jahr 2015, mehrere Hunderttausend Medizinprodukte hergestellt haben.

## DIE NT-TRADING GMBH & CO. KG IST MEHR ALS EIN HERSTELLER. DIE NT-TRADING GMBH & CO. KG REALISIERT SYSTEMLÖSUNGEN.

An unserer Fertigungsstätte in Karlsruhe realisieren wir sowohl die Produktentwicklung als auch die Fertigung in Eigenregie, um die für die anspruchsvollen nt-trading Produkte notwendigen nachhaltigen Qualitätsstandards zu gewährleisten,



die auf die Bedürfnisse unserer Kunden in aller Welt abgestimmt sind. Unsere Produkte werden aufwändig mit modernsten Fertigungsverfahren hergestellt. Damit sichern wir eine hohe Fertigungstiefe, die Voraussetzung für bestmögliche Herstellungs- und Verarbeitungsqualität. Alle Prozesse, von der Entwicklung bis zur Auslieferung, befinden sich unter einem Dach. Damit bekennen wir uns eindeutig zum Standort Deutschland, um von hier aus, die gewaltigen Qualitätsanforderungen der internationalen Dentalen Medizintechnikbranche zu erfüllen.

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# NT-TRADING EMPIRIE



Seit Beginn unserer Tätigkeit legen wir großen Wert auf eine konsequente Forschungs- und Entwicklungsarbeit in Kooperation mit renommierten Universitätskliniken und Instituten. Auf diese Weise gewährleisten wir die permanente Weiterentwicklung des Produktportfolios für die Dentale CAD/CAM Implantologie. Wir legen damit den Meilenstein, um den bestmöglichen Standard für unsere Anwender und ihre Patienten zu gewährleisten. Neben der Produktentwicklung engagiert sich Dirk Jahn, als Mitglieder des Richtlinienausschusses VDI 5705 „Digitale Prozessketten in der industriellen Medizintechnik“, für die Entwicklung nationaler Standards. Die einzigartigen nt-trading Produkte sind teilweise weltweit patentiert bzw. zum Patent angemeldet. Damit sichern wir das Potential, für zukünftige Weiterentwicklungen unserer Produkte und Anwendungsverfahren. Basierend auf unsere Kernkompetenz und des verbundenen Know-Hows „Made in Germany“ setzen wir gezielt auf die partnerschaftliche Förderung und Stärkung unserer weltweit agierenden Anwender.



## DYNAMISCHE PERSPEKTIVE

Dirk Jahn und Andreas Schütt haben als Geschäftsführende Gesellschafter die nt-trading Philosophie - Innovativ, Top-Qualität und Kundenorientiert - geprägt und zusammen mit ihren Mitarbeiterinnen und Mitarbeitern wird dieser weiter Dynamik mit zukunftsweisenden Produktinnovationen, mit weiteren spezialisierten und kompetenten Mitarbeitern und mit stetig verbessertem Kundenservice verliehen.

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

## **GUARANTEED SAFETY FOR YOU AND YOUR PATIENT**

Under our general terms of sales and delivery, we guarantee a perfect quality on our original nt-trading abutment components. Because of our high manufacturing and quality standards we can offer a warranty of 30 years on original nt-trading abutment components.

## **THE NT-TRADING WARRANTY CONTAINS:**

In case of a non-provisional prosthetic abutment component of nt-trading fails – nt-trading guarantees to replace that component with the same prosthetics abutment component of nt-trading for free.

## **IMPLANT WARRANTY**

Additionally nt-trading assumes an implant warranty of 30 years, but at maximum the one stated by the implant manufacturer.

## **FOR WHICH IMPLANTS DOES NT-TRADING ASSUMES A WARRANTY OF 30 YEARS?**

For implants on which original non-provisional nt-trading prosthetic components were processed after healing and for which the implant manufacturer rejects warranty for the reason that the implant was combined with original nt-trading components.


In case of warranty we refund the proven material costs for a new implant replacement. Further claims like operation- and/or laboratory costs cannot be assumed. A warranty can only be covered with our contracting party/purchaser (dentist, dental clinic, laboratory). Other parties cannot claim any rights of the warranty. The warranty claims cannot be assigned.

## **IN WHICH CASE WILL A WARRANTY NOT BE ASSUMED?**

- immediate restoration
- damage of our nt-trading abutment components or the implant due to external influences such force, accident, or non- professional treatment
- faulty material or manufacturing defects of the implant
- failure of our nt-trading abutment components or of the implant due to contraindications of the patient or due to alcoholism, smoking, drug consume or diabetes
- products, which have been custom-made or have been modified on the customer's' request



**Dirk Jahn, MDT, M.Sc.**  
Managing Director, Shareholder



**Andreas Schütt**  
Managing Director, Shareholder





## NT-TRADING LEBENSLANGE GARANTIE FÜR ABUTMENT PRODUKTE

### GARANTIEBEDINGUNGEN

Garantiert wird die Mangelfreiheit von nt-trading Abutment Produkten ab dem Zeitpunkt der Lieferung. Bei Vorliegen aller Garantiebedingungen wird von nt-trading das Abutment Produkt mit einem gleichen oder gleichwertigen Produkt kostenfrei ersetzt. Wenn ein Implantatanbieter seine Garantie aufgrund des Einsatzes eines nt-trading Abutments nicht erfüllt, deckt nt-trading sowohl das Abutment als auch das Implantat ab.

### ZEITRAUM DER GÜLTIGKEIT

Die Laufzeit der Garantie für nt-trading Abutment Produkte umfasst 30 Jahre ab Lieferdatum, bei fachgemäßer Handhabung und Ausführung: Mit der Garantieleistung ist keine neue Garantie oder Verlängerung der Garantie verbunden.

### GARANTIEUMFANG

Die nt-trading Garantie umfasst die kostenfreie Ersatzlieferung von nt-trading Abutment Produkten für CAD/CAM Implantat-Prothetik, für einen Zeitraum von bis zu 30 Jahre nach Auslieferung. Im Falle eines auf die von nt-trading gelieferte prothetische Komponente zurückzuführenden Implantatverlustes, stellt nt-trading, sollte dies aus zahnmedizinischen Gründen notwendig sein, ein kostenfreies Implantat. Wenn der Lieferant des Implantates den Ersatz des Implantates oder eine Kostenerstattung deshalb verweigert, weil ein nt-trading Abutment Produkt verwendet wurde, ist dies nt-trading durch ein entsprechendes Schreiben des Herstellers / Lieferanten zu belegen. Der Nachweis der Notwendigkeit im oben genannten Sinne obliegt dem Anwender. Die Letztentscheidung liegt bei nt-trading oder einem von dieser beauftragten Sachverständigen.

### VORAUSSETZUNGEN DER INANSPRUCHNAHME DER GARANTIE

Voraussetzung für die Inanspruchnahme der Garantie ist:

- I. Die Beachtung der zum Zeitpunkt des Anwendens vorliegenden Gebrauchsanweisungen von nt-trading und Materiallieferanten in Bezug auf alle nt-trading Produkte sowie der anerkannten zahntechnischen und zahnmedizinischen Verfahrensweisen vor, während und nach der Bearbeitung.
- II. Der Nachweis hierüber obliegt auf Nachfragen von nt-trading dem Anwender. Eine unsachgemäße Verwendung liegt beispielsweise vor, bei einer nicht fachgerechten Implantation, einer nicht fachgerechten Verschraubung des Abutments auf dem Implantat, einem Verstoß gegen die Vorgaben des jeweiligen Implantatherstellers (Lieferanten) für die Insertion des Implantates, insbesondere im Falle von Kontraindikationen, und äußere Einwirkungen wie Unfall oder vergleichbare Ereignisse. Für die jeweiligen Implantatsysteme sind die nt-trading Verarbeitungsanleitungen und Gebrauchsanweisungen maßgeblich für die Beurteilung des Reklamationsfalles. Die Fertigungsparameter für die nt-trading Abutment Produkte sind einzuhalten und es darf für das beanstandete Produkt keine Sonderfreigabe zur Produktion erteilt worden sein.
- III. Die Einreichung eines ausgefüllten und unterschriebenen Reklamationsformulars spätestens drei Monate nach Auftreten eines Garantiefalles.
- IV. Kopie der Zurückweisung des Garantieanspruchs durch den Hersteller des entsprechenden Implantats.
- V. Die Rücksendung des beanstandeten nt-trading Produktes im gereinigten und desinfizierten Zustand.

### ABGRENZUNGEN UND BESCHRÄNKUNGEN

Die nt-trading Garantie ist eine gesonderte Garantie von nt-trading und tritt neben die Gewährleistungsrechte aus dem Liefervertrag in Abhängigkeit zu unseren Allgemeinen Geschäftsbedingungen. Die vertraglichen oder gesetzlichen Rechte des Anwenders werden durch diese Garantie nicht berührt.

### ANWENDUNGSGEBIET

Diese kostenfreie nt-trading Garantie gilt nur für nt-trading Abutment Produkte, die von nt-trading in der Bundesrepublik Deutschland verkauft worden sind >>Anwendungsgebiet<< Die Garantiebedingungen gelten bis auf Widerruf für alle entsprechenden Lieferungen. Die Beurteilung des Vorliegens eines Garantiefalles obliegt auf der Grundlage der vorstehenden Garantiebedingungen der Firma nt-trading GmbH & Co. KG oder einem von dieser beauftragten Sachverständigen. Die Entscheidung von nt-trading GmbH & Co. KG oder dem von dieser beauftragten Sachverständigen ist für die Parteien verbindlich. Diese Garantie unterliegt dem Recht der Bundesrepublik Deutschland.

Alle Unterlagen sind einzureichen bei: **nt-trading GmbH & Co. KG, G.-Braun-Str. 18, 76187 Karlsruhe, Germany**

### AGB

Es gelten die **allgemeinen Geschäftsbedingungen (AGB)** der **nt-trading GmbH & Co. KG Deutschland**. Die ausführlichen AGB finden Sie auf unserer Website unter: [http://www.nt-trading.com/agb\\_de.pdf](http://www.nt-trading.com/agb_de.pdf)



**Dirk Jahn, MDT, M.Sc.**  
Managing Director, Shareholder



**Andreas Schütt**  
Managing Director, Shareholder



# TABLE OF CONTENTS

## 1 TITANIUM BASE ABUTMENT

### IMPLANT SYSTEMS

#### BEG-SERIES – NEW

is compatible to: BEGO Implant Systems® / Semados®  
S, RS-RX, RI-Line - - - - - 12

#### BIO-SERIES – NEW

is compatible to: BioHorizons® / internal - - - - - 13

#### BRE-SERIES – NEW

is compatible to: Bredent Medical® / Sky® - - - - - 14

#### CAM-SERIES

is compatible to: Altatec® / Camlog® - - - - - 15

#### COL-SERIES

is compatible to: Altatec® / Conelog® - - - - - 16

#### E-SERIES

is compatible to: Nobel Biocare™ / Replace Select® - - - - - 17

#### F-SERIES

is compatible to: Nobel Biocare™ / Nobel Active™ - - - - - 21

#### H-SERIES

is compatible to: Biomet 3i® / Certain® - - - - - 22

#### HIO-SERIES – NEW

is compatible to: HIOSSEN® / OSSTEM TS® - - - - - 23

#### I-SERIES

is compatible to: Biomet 3i® / Osseotite® External Hex® - 24

#### K-SERIES

is compatible to: Nobel Biocare™ / Brånemark® - - - - - 25

#### L-SERIES

is compatible to: Straumann / Bone Level® - - - - - 26

#### MEX-SERIES – NEW

is compatible to: Medentis Medical® / ICX® - - - - - 29

#### MIC-SERIES – NEW

is compatible to: MIS® / C1® - - - - - 30

#### MIS-SERIES – NEW

is compatible to: MIS® / SEVEN® - - - - - 31

#### N-SERIES

is compatible to: Straumann / SynOcta® - - - - - 32

#### NEO-SERIES – NEW

is compatible to: NEOSS Implant System® / NEOSS™ - - - - 35

#### R-SERIES

is compatible to: Zimmer Dental / Tapered Screw-Vent® - 36

#### S-SERIES

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System OsseoSpeed® TX - - - - - 39

#### SEV-SERIES – NEW

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System™ EV - - - - - 42

#### T-SERIES

is compatible to: DENTSPLY Implants® / Xive® - - - - - 43

#### THO-SERIES – NEW

is compatible to: Thommen Medical® / SPI® - - - - - 46

#### UPR-SERIES – NEW

is compatible to: Sweden & Martina Implantology™ /  
Premium Kohno® - - - - - 47

#### UTG-SERIES – NEW

is compatible to: Sweden & Martina Implantology™ /  
Premium TG® - - - - - 48

## 2 2-CONnect® ABUTMENT

### IMPLANT SYSTEMS

#### BEG-SERIES – NEW

is compatible to: BEGO Implant Systems® / Semados®  
S, RS-RX, RI-Line - - - - - 52

#### BIO-SERIES – NEW

is compatible to: BioHorizons® / internal - - - - - 55

#### BRE-SERIES – NEW

is compatible to: Bredent Medical® / Sky® - - - - - 58

#### CAM-SERIES

is compatible to: Altatec® / Camlog® - - - - - 61

#### COL-SERIES – NEW

is compatible to: Altatec® / Conelog® - - - - - 64

#### E-SERIES

is compatible to: Nobel Biocare™ / Replace Select® - - - - - 67

#### F-SERIES

is compatible to: Nobel Biocare™ / Nobel Active™ - - - - - 70

#### H-SERIES

is compatible to: Biomet 3i® / Certain® - - - - - 73

#### HIO-SERIES – NEW

is compatible to: HIOSSEN® / OSSTEM TS® - - - - - 76

#### L-SERIES

is compatible to: Straumann / Bone Level® - - - - - 79

#### MEX-SERIES – NEW

is compatible to: Medentis Medical® / ICX® - - - - - 82

#### MIC-SERIES – NEW

is compatible to: MIS® / C1® - - - - - 85

#### MIS-SERIES – NEW

is compatible to: MIS® / SEVEN® - - - - - 88

#### N-SERIES

is compatible to: Straumann / SynOcta® - - - - - 91

#### NEO-SERIES – NEW

is compatible to: NEOSS Implant System® / NEOSS™ - - - - 94

#### R-SERIES

is compatible to: Zimmer Dental / Tapered Screw-Vent® - 97

#### S-SERIES

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System OsseoSpeed® TX - - - - - 100

#### SEV-SERIES – NEW

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System™ EV - - - - - 103

#### T-SERIES

is compatible to: DENTSPLY Implants® / Xive® - - - - - 106

#### THO-SERIES – NEW

is compatible to: Thommen Medical® / SPI® - - - - - 109

#### UPR-SERIES – NEW

is compatible to: Sweden & Martina Implantology™ /  
Premium Kohno® - - - - - 112

#### UTG-SERIES – NEW

is compatible to: Sweden & Martina Implantology™ /  
Premium TG® - - - - - 115

### 3 NT-PREFORMS® ABUTMENT

#### IMPLANT SYSTEMS

##### BEG-SERIES – NEW

is compatible to: BEGO Implant Systems® / Semados®  
S, RS-RX, RI-Line - - - - - 120

##### BIO-SERIES – NEW

is compatible to: BioHorizons® / internal - - - - - 121

##### BRE-SERIES – NEW

is compatible to: Bredent Medical® / Sky® - - - - - 122

##### CAM-SERIES

is compatible to: Altatec® / Camlog® - - - - - 123

##### COL-SERIES

is compatible to: Altatec® / Conelog® - - - - - 124

##### E-SERIES

is compatible to: Nobel Biocare™ / Replace Select® - - - - - 125

##### F-SERIES

is compatible to: Nobel Biocare™ / Nobel Active™ - - - - - 126

##### I-SERIES

is compatible to: Biomet 3i® / Osseotite® External Hex® - 126

##### H-SERIES

is compatible to: Biomet 3i® / Certain® - - - - - 127

##### HIO-SERIES – NEW

is compatible to: HIOSSEN® / OSSTEM TS® - - - - - 128

##### K-SERIES

is compatible to: Nobel Biocare™ / Brånemark® - - - - - 129

##### L-SERIES

is compatible to: Straumann / Bone Level® - - - - - 130

##### MEX-SERIES – NEW

is compatible to: Medentis Medical® / ICX® - - - - - 131

##### MIC-SERIES – NEW

is compatible to: MIS® / C1® - - - - - 132

##### MIS-SERIES – NEW

is compatible to: MIS® / SEVEN® - - - - - 133

##### N-SERIES

is compatible to: Straumann / SynOcta® - - - - - 134

##### NEO-SERIES – NEW

is compatible to: NEOSS Implant System® / NEOSS™ - - - - - 135

##### R-SERIES

is compatible to: Zimmer Dental / Tapered Screw-Vent® - 136

##### S-SERIES

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System OsseoSpeed® TX - - - - - 137

##### SEV-SERIES – NEW

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System™ EV - - - - - 138

##### T-SERIES

is compatible to: DENTSPLY Implants® / Xive® - - - - - 139

##### THO-SERIES – NEW

is compatible to: Thommen Medical® / SPI® - - - - - 140

##### UPR-SERIES – NEW

is compatible to: Sweden & Martina Implantology™ /  
Premium Kohno® - - - - - 141

##### UTG-SERIES – NEW

is compatible to: Sweden & Martina Implantology™ /  
Premium TG® - - - - - 142

#### Holder fixture and Accessories

• Holder fixture - - - - -	143
• Accessories - - - - -	144
• 3,5 mm Abutment grip - - - - -	145
• 4,3 mm Abutment grip - - - - -	146
• 5,0 mm Abutment grip - - - - -	147

### 4 DIM ANALOG

#### All IMPLANT SYSTEMS

Digital-Implant-Model Analog (DIM) - - - - -	148
--	-----

### 5 SURGICAL GUIDE SLEEVES

#### IMPLANT SYSTEMS

Surgical Guide Sleeves - - - - -	164
----------------------------------	-----

### 6 TOOLS & DISCS

#### All IMPLANT SYSTEMS

Prosthetic tools - - - - -	168
Surgical Guide Sleeve Tools - - - - -	174
Sinter components - - - - -	175
Dentokeep PEEK Disc- - - - -	176
DENTOMODEL - - - - -	178
Scan Equipment - - - - -	180
nt-milling tools & grinding tools- - - - -	181

### 7 NT-iDent

#### All IMPLANT SYSTEMS

Technology center info- - - - -	184
---------------------------------	-----

### 8 SPECIFICATION

#### All IMPLANT SYSTEMS

Tightening torques - - - - -	190
------------------------------	-----

# TITANIUM BASE

*For implant supported individual hybrid abutments*



## **BENEFITS:**

- engaged
- for individual abutment design
- large glue surface, so durable solid connection to the base
- conventional usable and also for CAD/CAM process



## **APPLICATION:**

- for individual glued ceramic abutments (zirconia, lithiumdisilicate) or synthetics (PMMA, PEEK, composite)



## **TECHNICAL DETAILS:**

- Titanium Grade 5 ELI



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# TABLE OF CONTENTS

NT CATALOGUE 2017-1

<b>1</b>	<b>TITANIUM BASE ABUTMENT</b>	<b>10 – 49</b>
<b>2</b>	<b>2-CONnect® ABUTMENT</b>	<b>50 – 117</b>
<b>3</b>	<b>NT-PREFORMS® ABUTMENT</b>	<b>118 – 147</b>
<b>4</b>	<b>DIM ANALOG</b>	<b>148 – 161</b>
<b>5</b>	<b>SURGICAL GUIDE SLEEVES</b>	<b>163 – 165</b>
<b>6</b>	<b>TOOLS &amp; DISCS</b>	<b>167 – 181</b>
<b>7</b>	<b>NT-iDent</b>	<b>182 – 189</b>
<b>8</b>	<b>SPECIFICATION</b>	<b>190 – 191</b>

## **BEG-SERIES – NEW**

is compatible to: BEGO Implant Systems® / Semados®  
S, RS-RX, RI-Line - - - - - **12**

## **BIO-SERIES – NEW**

is compatible to: BioHorizons® / internal- - - - - **13**

## **BRE-SERIES – NEW**

is compatible to: Bredent Medical® / Sky® - - - - - **14**

## **CAM-SERIES**

is compatible to: Altatec® / Camlog® - - - - - **15**

## **COL-SERIES**

is compatible to: Altatec® / Conelog® - - - - - **16**

## **E-SERIES**

is compatible to: Nobel Biocare™ / Replace Select®- - - - - **17**

## **F-SERIES**

is compatible to: Nobel Biocare™ / Nobel Active™ - - - - - **21**

## **H-SERIES**

is compatible to: Biomet 3i® / Certain® - - - - - **22**

## **HIO-SERIES – NEW**

is compatible to: HIOSSSEN® / OSSTEM TS® - - - - - **23**

## **I-SERIES**

is compatible to: Biomet 3i® / Osseotite® External Hex® - - **24**

## **K-SERIES**

is compatible to: Nobel Biocare™ / Brånemark® - - - - - **25**

## **L-SERIES**

is compatible to: Straumann / Bone Level®- - - - - **26**

## **MEX-SERIES – NEW**

is compatible to: Medentis Medical® / ICX®- - - - - **29**

## **MIC-SERIES – NEW**

is compatible to: MIS® / C1® - - - - - **30**

## **MIS-SERIES – NEW**

is compatible to: MIS® / SEVEN®- - - - - **31**

## **N-SERIES**

is compatible to: Straumann / SynOcta® - - - - - **32**

## **NEO-SERIES – NEW**

is compatible to: NEOSS Implant System® / NEOSS™ - - - - - **35**

## **R-SERIES**

is compatible to: Zimmer Dental / Tapered Screw-Vent® - - **36**

## **S-SERIES**

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System OsseoSpeed® TX - - - - - **39**

## **SEV-SERIES – NEW**

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System™ EV - - - - - **42**

## **T-SERIES**

is compatible to: DENTSPLY Implants® / Xive® - - - - - **43**

## **THO-SERIES – NEW**

is compatible to: Thommen Medical® / SPI® - - - - - **46**

## **UPR-SERIES – NEW**

is compatible to: Sweden & Martina Implantology™ /  
Premium Kohno®- - - - - **47**

## **UTG-SERIES – NEW**

is compatible to: Sweden & Martina Implantology™ /  
Premium TG®- - - - - **48**



# BEG-SERIES

compatible to: BEGO Implant Systems® / Semados® S, RS-RX, RI-Line



**PLATFORM**

3,25 / 3,75 mm

4,1 mm

4,5 mm

5,5 mm

**TITANIUM BASE**

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



BEG 80323700

BEG 80410000

BEG 80450000

BEG 80550000

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



BEG 9.S3D3.237

BEG 9.S3D4.100

BEG 9.S3D4.500

BEG 9.S3D5.500

★

**NT-MILL LAB ANALOG**

Stainless Steel



BEG 5.La3.237

BEG 5.La4.100

BEG 5.La4.500

BEG 5.La5.500

★

**IMPLANT PICK-UP**

for open-tray with  
integrated screw  
Coming soon



BEG TR-00013.2

BEG TR-00024.1

BEG TR-00034.5

BEG TR-00045.5

**ABUTMENT SCREW**

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



BEG 603255

BEG 603255

BEG 603255

BEG 603255

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# BIO-SERIES

compatible to: BioHorizons® / internal



**PLATFORM**

3,0 mm      3,5 mm      4,5 mm      5,7 mm

**TITANIUM BASE**

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



BIO 8030000      BIO 8035000      BIO 8045000      BIO 8057000

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



BIO 9.S3D3.000      BIO 9.S3D3.500      BIO 9.S3D4.500      BIO 9.S3D5.700 ★

**NT-MILL LAB ANALOG**


Stainless Steel



BIO 5.La3.000      BIO 5.La3.500      BIO 5.La4.500      BIO 5.La5.700 ★

**IMPLANT PICK-UP**

for open-tray with  
integrated screw  
*Coming soon*



BIO TR-00013.0      BIO TR-00023.5      BIO TR-00034.5      BIO TR-00045.7

**ABUTMENT SCREW**

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



BIO 603057      BIO 603057      BIO 603057      BIO 603057

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 🇺🇸

# BRE-SERIES

compatible to: Bredent Medical® / Sky®



**PLATFORM**

3,5 mm

4,0 mm

**TITANIUM BASE**

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



BRE 80350000

BRE 80400000

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



BRE 9.S3D3.500

BRE 9.S3D4.000

★

**NT-MILL LAB ANALOG**

Stainless Steel



BRE 5.La3.500

BRE 5.La4.000

★

**IMPLANT PICK-UP**

for open-tray with  
integrated screw  
Coming soon



BRE TR-00013.5

BRE TR-00024.0

**ABUTMENT SCREW**

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



BRE 603540

BRE 603540

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# CAM-SERIES

compatible to: Altatec® / Camlog®



## PLATFORM

3,3 mm

3,8 mm

4,3 mm

5,0 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screws  
Titanium Grade 5 ELI



CAM 80330000

CAM 80380000

CAM 80430000

CAM 80500000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



CAM 9.S3D3.300

CAM 9.S3D3.800

CAM 9.S3D4.300

CAM 9.S3D5.060

★

## NT-MILL LAB ANALOG

Stainless Steel



CAM 5.La3.300

CAM 5.La3.800

CAM 5.La4.300

CAM 5.La5.060

★

## IMPLANT PICK-UP

for open-tray with  
integrated screw  
Coming soon



CAM TR-00013.3

CAM TR-00023.8

CAM TR-00034.3

—

## LAB SCREW

coloured screw



CAM 6233843

CAM 6233843

CAM 6233843

CAM 6250600

★

## ABUTMENT SCREW

Recommended tightening  
torques 20 Ncm  
Titanium Grade 5 ELI



CAM 6033843

CAM 6033843

CAM 6033843

CAM 6150600

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# COL-SERIES

compatible to: Altatec® / Conelog®



## PLATFORM

3,3 mm

3,8 / 4,3 mm

5,0 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screws  
Titanium Grade 5 ELI



Gingiva Height ..... 0,8 mm  
..... 2,0 mm

COL 80330008

COL 80384308

COL 80500008

COL 80330020

COL 80384320

COL 80500020

## SCAN BODY

for Titanium Base  
incl. coloured lab screw  
PEEK



COL 703300

COL 703843

COL 705000

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



COL 9.S3D3.300

COL 9.S3D3.843

COL 9.S3D5.000

★

## NT-MILL LAB ANALOG

Stainless Steel



COL 5.La3.300

COL 5.La3.843

COL 5.La5.000

★

## IMPLANT PICK-UP

for open-tray with  
integrated screw  
Coming soon



COL TR-00013.3

COL TR-00023.8

—

## LAB SCREW

coloured screw



COL 623343

COL 623343

COL 625000

## ABUTMENT SCREW

Recommended tightening  
torques 20 Ncm  
Titanium Grade 5 ELI



COL 603343

COL 603343

COL 605000

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# E-SERIES

compatible to: Nobel Biocare™ / Replace Select®



## PLATFORM

3,5 mm NP

4,3 mm RP

5,0 mm WP

6,0 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



E 800

E 810

E 820

E 830

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



E 9.S3D3.500

E 9.S3D4.300

E 9.S3D5.000

E 9.S3D6.000

★

## LAB ANALOG

Stainless Steel



E 50

E 51

E 52

E 53

★

## IMPLANT PICK-UP

for open-tray with  
integrated screw



E TR-NP013.5

E TR-RP024.3

E TR-WP035.0

—

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



E 60

E 61

E 61

E 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# E-SERIES

compatible to: Nobel Biocare™ / Replace Select®



## PLATFORM

3,5 mm NP

4,3 mm RP

5,0 mm WP

## STRAIGHT ABUTMENT

Gingiva Height 1,0 mm  
incl. screw  
Titanium Grade 5 ELI



E 100-1

E 110-1

E 120-1

★

## STRAIGHT ABUTMENT

Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



E 100

E 110

E 120

★

## UCLA ABUTMENT

engaging  
incl. screw



E 11.CA3.500

E 11.CA4.300

E 11.CA5.000

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



E 60

E 61

E 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# E-SERIES

compatible to: Nobel Biocare™ / Replace Select®



## PLATFORM

3,5 mm NP

4,3 mm RP

5,0 mm WP

### ANGLED ABUTMENT 16°

angled over surface  
Gingiva Height 1,0 mm  
incl. screw  
Titanium Grade 5 ELI



E 200-1-1

E 210-1-1

E 220-1-1

### ANGLED ABUTMENT 16°

angled over edge  
Gingiva Height 1,0 mm  
incl. screw  
Titanium Grade 5 ELI



E 200-2-1

E 210-2-1

E 220-2-1

### ANGLED ABUTMENT 16°

angled over surface  
Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



E 200-1

E 210-1

E 220-1

### ANGLED ABUTMENT 16°

angled over edge  
Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



E 200-2

E 210-2

E 220-2

### ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



E 60

E 61

E 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# 3D-Guide®

Scanbody for high-precision implant position transfer



## BENEFITS:

- exact positioning by metal interface
- conceived for intra-oral scanners
- the different shape geometry ensured in case of incomplete scanning detection a perfect transfer in CAD software
- screw integrated
- x-ray detectable
- rotatable in case of dental crowding



## APPLICATION:

- scanbody for model scanning
- scanbody for oral scanning



## TECHNICAL DETAILS:

- tolerance 2–3 µm



**INTERNATIONAL  
PATENT**



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with \* are available in the USA 

# F-SERIES

compatible to: Nobel Biocare™ / Nobel Active™



## PLATFORM

3,5 mm NP

4,3 / 5,0 mm RP

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



F 800

F 810



## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



F 9.S3D3.500

F 9.S3D4.350



## LAB ANALOG

Stainless Steel



F 50

F 51



## IMPLANT PICK-UP

for open-tray with  
integrated screw  
Coming soon



F TR-NP013.5

F TR-RP024.3

## ABUTMENT SCREW

Recommended tightening  
torques: NP = 25 Ncm  
RP = 35 Ncm  
Titanium Grade 5 ELI



F 60

F 61



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# H-SERIES

compatible to: Biomet 3i® / Certain®



## PLATFORM

3,4 mm NP

4,1 mm RP

5,0 mm WP

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



H 800

H 810

H 820



## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



H 9.S3D3.400

H 9.S3D4.150

H 9.S3D4.150



## LAB ANALOG

Stainless Steel



H 50

H 51

H 52



## IMPLANT PICK-UP

for open-tray with  
integrated screw

Coming soon



H TR-NP013.4

H TR-RP024.1

H TR-WP035.0

## ABUTMENT SCREW

Recommended tightening  
torques 20 Ncm

Titanium Grade 5 ELI



H 60

H 60

H 60



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# HIO-SERIES

compatible to: HIOSSEN® / OSSTEM TS®



**PLATFORM**

3,5 mm

4,0 - 6,0 mm

**TITANIUM BASE**

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



HIO 80350000

HIO 80406000

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



HIO 9.S3D3.500

HIO 9.S3D4.060

★

**NT-MILL LAB ANALOG**

Stainless Steel



HIO 5.La3.500

HIO 5.La4.060

★

**IMPLANT PICK-UP**

for open-tray with  
integrated screw

Coming soon



HIO TR-00013.5

HIO TR-00024.0

**ABUTMENT SCREW**

Recommended tightening  
torques 3,5 mm = 20 Ncm  
4,0 - 6,0 mm = 30 Ncm  
Titanium Grade 5 ELI



HIO 603500

HIO 604060

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 🇺🇸

# I-SERIES

compatible to: Biomet 3i® / Osseotite® External Hex®



## PLATFORM

3,4 mm

4,1 mm

5,0 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



I 800

I 810

I 820



## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



I 9.S3D3.400

I 9.S3D4.150

I 9.S3D4.150



## LAB ANALOG

Stainless Steel



I 50

I 51

I 52



## STRAIGHT ABUTMENT

Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



—

I 110

—



## IMPLANT PICK-UP

for open-tray with  
integrated screw  
Coming soon



I TR-00013.4

I TR-00024.1

—

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



I 61

I 61

I 61



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# K-SERIES

compatible to: Nobel Biocare™ / Brånemark®



## PLATFORM

3,5 mm

4,1 mm

5,1 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



K 800

K 810

K 820

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



K 9.S3D3.500

K 9.S3D4.100

K 9.S3D5.100

★

## LAB ANALOG

Stainless Steel



K 50

K 51

K 52

★

## STRAIGHT ABUTMENT

Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



—

K 110

—

★

## IMPLANT PICK-UP

for open-tray with  
integrated screw  
Coming soon



K TR-00013.5

K TR-00024.1

—

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



K 60

K 61

K 62

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# L-SERIES

compatible to: Straumann / Bone Level®



## PLATFORM

3,3 mm NC

4,1 / 4,8 mm RC

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



L 800

L 810

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



L 9.S3D3.300

L 9.S3D4.148

★

## LAB ANALOG

Stainless Steel



L 50

L 51

★

## IMPLANT PICK-UP

for open-tray with  
integrated screw



L TR-NC013.3

L TR-RC024.1

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



L 60

L 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# L-SERIES

compatible to: Straumann / Bone Level®



## PLATFORM

3,3 mm NC

4,1 / 4,8 mm RC

## STRAIGHT ABUTMENT

Gingiva Height 1,5 mm  
incl. screw  
Titanium Grade 5 ELI



L 100

L 110

## STRAIGHT ABUTMENT

Gingiva Height 3,0 mm  
incl. screw  
Titanium Grade 5 ELI



L 100-3

L 110-3

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



L 60

L 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# L-SERIES

compatible to: Straumann / Bone Level®



## PLATFORM

3,3 mm NC

4,1 / 4,8 mm RC

### ANGLED ABUTMENT 18°

angled over surface  
Gingiva Height 1,5 mm  
incl. screw  
Titanium Grade 5 ELI



L 200-1

L 210-1

### ANGLED ABUTMENT 18°

angled over edge  
Gingiva Height 1,5 mm  
incl. screw  
Titanium Grade 5 ELI



L 200-2

L 210-2

### ANGLED ABUTMENT 18°

angled over surface  
Gingiva Height 3,0 mm  
incl. screw  
Titanium Grade 5 ELI



L 200-1-3

L 210-1-3

### ANGLED ABUTMENT 18°

angled over edge  
Gingiva Height 3,0 mm  
incl. screw  
Titanium Grade 5 ELI



L 200-2-3

L 210-2-3

### ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



L 60

L 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# MEX-SERIES

compatible to: Medentis Medical® / ICX®



## PLATFORM

3,45 - 4,8 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



MEX 80374800

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



MEX 9.S3D3.748



## NT-MILL LAB ANALOG

Stainless Steel



MEX 5.La3.748



## IMPLANT PICK-UP

for open-tray with  
integrated screw  
Coming soon



MEX TR-00013.7

## ABUTMENT SCREW

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



MEX 603748

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# MIC-SERIES

compatible to: MIS® / C1®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**TITANIUM BASE**

for individual milled Zirconium Abutment incl. screw  
Titanium Grade 5 ELI



MIC 80330000

MIC 80374200

MIC 80500000

**SCAN BODY 3D-GUIDE®**

for intra + extra oral scanning



MIC 9.S3D3.300

MIC 9.S3D3.742

MIC 9.S3D5.000

★

**NT-MILL LAB ANALOG**

Stainless Steel



MIC 5.La3.300

MIC 5.La3.742

MIC 5.La5.000

★

**IMPLANT PICK-UP**

for open-tray with integrated screw  
Coming soon



MIC TR-00013.3

MIC TR-00023.7

MIC TR-00035.0

**ABUTMENT SCREW**

Recommended tightening torques 30 Ncm  
Titanium Grade 5 ELI



MIC 603300

MIC 603750

MIC 603750

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA



# MIS-SERIES

compatible to: MIS® / SEVEN®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**TITANIUM BASE**

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



MIS 80330000

MIS 80374200

MIS 80500000

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



MIS 9.S3D3.300



MIS 9.S3D3.742

MIS 9.S3D5.000

★

**NT-MILL LAB ANALOG**

Stainless Steel



MIS 5.La3.300

MIS 5.La3.742

MIS 5.La5.000

★

**IMPLANT PICK-UP**

for open-tray with  
integrated screw  
Coming soon



MIS TR-00013.3

MIS TR-00023.7

MIS TR-00035.0

**ABUTMENT SCREW**

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



MIS 603300

MIS 603750

MIS 603750

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 🇺🇸

# N-SERIES

compatible to: Straumann / SynOcta®



## PLATFORM

3,5 mm NN

4,8 mm RN

6,5 mm WN

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



N 80

N 810

N 820

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



N 9.S3D3.500

N 9.S3D4.800

N 9.S3D6.500

★

## LAB ANALOG

Stainless Steel



N 50

N 51

N 52

★

## IMPLANT PICK-UP

for open-tray with  
integrated screw



N TR-NN013.5

N TR-RN024.8

N TR-WN036.5

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



N 60

N 62

N 62

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# N-SERIES

compatible to: Straumann / SynOcta®



## PLATFORM

3,5 mm NN

4,8 mm RN

4,8 mm RN

6,5 mm WN

## STRAIGHT ABUTMENT


incl. screw

Titanium Grade 5 ELI




Gingiva Height  
2,5 mm

N 100




Body height  
5,0 mm

N 110



Body height  
6,5 mm

N 110 L



Body height  
4,0 mm

N 120

★

## ANGLED ABUTMENT 16°

angled over surface

Gingiva Height 2,5 mm

incl. screw

Titanium Grade 5 ELI



N 210-1



N 220-1

## ANGLED ABUTMENT 16°

angled over edge

Gingiva Height 2,5 mm

incl. screw

Titanium Grade 5 ELI



N 200



N 210-2



N 220-2

## ANGLED ABUTMENT 21°

angled over surface

Gingiva Height 2,5 mm

incl. screw

Titanium Grade 5 ELI



N 210-1-21

## ANGLED ABUTMENT 21°

angled over edge

Gingiva Height 2,5 mm

incl. screw

Titanium Grade 5 ELI



N 210-2-21

## STRAIGHT MASSIV ABUTMENT

incl. 2 screws

Titanium Grade 5 ELI



N 410

## ABUTMENT SCREW

Recommended tightening

torques 35 Ncm

Titanium Grade 5 ELI



N 60



N 61



N 61



N 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# N-SERIES

compatible to: Straumann / SynOcta®



## PLATFORM

3,5 mm NN

4,8 mm RN

6,5 mm WN

## UCLA ABUTMENT

engaging  
incl. screw



N 300

—

N 320

## UCLA ABUTMENT

non-engaging  
incl. screw



N 300 R

—

N 320 R

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



N 60

N 62

N 62

★

 Platform 4,8 mm RN

## RN-MASSIV ABUTMENT

Recommended tightening  
torques 35 Ncm  
only for dentist  
Titanium Grade 5 ELI

Body height  
4,0 mm

Body height  
5,5 mm

Body height  
7,0 mm



N 110-40

N 110-55

N 110-70

★

 Platform 6,5 mm WN

## WN-MASSIV ABUTMENT

Recommended tightening  
torques 35 Ncm  
only for dentist  
Titanium Grade 5 ELI

Body height  
4,0 mm

Body height  
5,5 mm



N 120-40

N 120-55


—

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# NEO-SERIES

compatible to: *NEOSS Implant System*<sup>®</sup> / *NEOSS*<sup>™</sup>



## PLATFORM

3,5 - 5,5 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



NEO 80355500

## SCAN BODY 3D-GUIDE<sup>®</sup>

for intra + extra  
oral scanning



NEO 9.S3D3.555



## NT-MILL LAB ANALOG

Stainless Steel



NEO 5.La3.555



## IMPLANT PICK-UP

for open-tray with  
integrated screw  
Coming soon



NEO TR-00013.5

## ABUTMENT SCREW

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



NEO 603555

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# R-SERIES

compatible to: Zimmer Dental / Tapered Screw-Vent®



## PLATFORM

3,5 mm

4,5 mm

5,7 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



R 800

R 810

R 820



## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



R 9.S3D3.500

R 9.S3D4.500

R 9.S3D5.700



## LAB ANALOG

Stainless Steel



R 50

R 51

R 52



## IMPLANT PICK-UP

for open-tray with  
integrated screw



R TR-00013.5

R TR-00024.5

—

## ABUTMENT SCREW

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



R 60

R 60

R 60



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# R-SERIES

compatible to: Zimmer Dental / Tapered Screw-Vent®



## PLATFORM

3,5 mm

4,5 mm

5,7 mm

## STRAIGHT ABUTMENT

Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



R 100

R 110

R 120



## ANGLED ABUTMENT 16°

angled over surface  
Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



R 200-1

R 210-1

R 220-1

## ANGLED ABUTMENT 16°

angled over edge  
Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



R 200-2

R 210-2

R 220-2

## MASSIV ABUTMENT

incl. 2 screws  
Titanium Grade 5 ELI



R 400

R 410

R 420



## ABUTMENT SCREW

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



R 60

R 60


R 60



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# R-SERIES

compatible to: Zimmer Dental / Tapered Screw-Vent®



## PLATFORM

3,5 mm

4,5 mm

5,7 mm

## UCLA ABUTMENT

engaging  
incl. screw



—

R 310

R 320

## UCLA ABUTMENT

non-engaging  
incl. screw



R 300-R

R 310-R

R 320-R

## ABUTMENT SCREW

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



R 60

R 60

R 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# S-SERIES

compatible to: DENTSPLY Implants® / Astra Tech Implant System OsseoSpeed® TX



## PLATFORM

3,5 / 4,0 mm

4,5 / 5,0 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



S 800

S 820



## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



S 9.S3D3.540

S 9.S3D4.550



## LAB ANALOG

Stainless Steel



S 50

S 52



## IMPLANT PICK-UP

for open-tray with  
integrated screw



S TR-00013.5

S TR-00024.5

## ABUTMENT SCREW

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



S 60

S 61



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# S-SERIES

compatible to: DENTSPLY Implants® / Astra Tech Implant System OsseSpeed® TX



**PLATFORM**


3,5 / 4,0 mm

3,5 / 4,0 mm

4,5 / 5,0 mm

**STRAIGHT ABUTMENT**

Gingiva Height 1,5 mm  
incl. screw  
Titanium Grade 5 ELI



S 100

S 110

S 120

★

**STRAIGHT ABUTMENT**

Gingiva Height 3,0 mm  
incl. screw  
Titanium Grade 5 ELI



S 100-3

S 110-3

S 120-3

★

**ANGLED ABUTMENT 16°**

angled over surface  
Gingiva Height 1,5 mm  
incl. screw  
Titanium Grade 5 ELI



S 200

S 210

S 220

**ANGLED ABUTMENT 16°**

angled over surface  
Gingiva Height 3,0 mm  
incl. screw  
Titanium Grade 5 ELI



S 200-3

S 210-3

S 220-3

**ABUTMENT SCREW**

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



S 60

S 60

S 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# S-SERIES

compatible to: DENTSPLY Implants® / Astra Tech Implant System OsseoSpeed® TX



## PLATFORM

3,5 / 4,0 mm

4,5 / 5,0 mm

## STRAIGHT MASSIV ABUTMENT

incl. 2 screws

Titanium Grade 5 ELI



S 400

S 420

★

## UCLA ABUTMENT

engaging

incl. screw



S 11.CA3.540

S 11.CA4.550

## ABUTMENT SCREW

Recommended tightening

torques 25 Ncm

Titanium Grade 5 ELI



S 60

S 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
 Products indicated with ★ are available in the USA 🇺🇸

# SEV-SERIE

compatible to: DENTSPLY Implants® / Astra Tech Implant System™ EV




**PLATFORM**

3,0 mm      3,6 mm      4,2 mm      4,8 mm      5,4 mm

**TITANIUM BASE**

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



SEV 80300000      SEV 80360000      SEV 80420000      SEV 80480000      SEV 80540000

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



SEV 9.S3D3.000      SEV 9.S3D3.600      SEV 9.S3D4.200      SEV 9.S3D4.800      SEV 9.S3D5.400 ★

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



SEV 5.La3.000      SEV 5.La3.600      SEV 5.La4.200      SEV 5.La4.800      SEV 5.La5.400 ★

**IMPLANT PICK-UP**

for open-tray with  
integrated screw  
Coming soon



SEV TR-00013.0      SEV TR-00023.6      SEV TR-00034.2      SEV TR-00044.8      SEV TR-00055.4

**ABUTMENT SCREW**

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



SEV 603000      SEV 603600      SEV 604200      SEV 604854      SEV 604854

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# T-SERIES

compatible to: DENTSPLY Implants® / Xive®



## PLATFORM

3,4 mm

3,8 mm

4,5 mm

5,5 mm

## TITANIUM BASE

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



T 800

T 805

T 810

T 820



## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



T 9.S3D3.400

T 9.S3D3.800

T 9.S3D4.555

T 9.S3D4.555



## LAB ANALOG

Stainless Steel



T 50

T 55

T 51

T 52



## IMPLANT PICK-UP

for open-tray with  
integrated screw



T TR-00013.4

T TR-00023.8

T TR-00034.5

—

## ABUTMENT SCREW

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



T 60

T 60

T 60

T 60



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# T-SERIES

compatible to: DENTSPLY Implants® / Xive®



3,4 mm



3,8 mm



4,5 mm



5,5 mm

## PLATFORM

### STRAIGHT ABUTMENT

Gingiva Height 1,0 mm  
incl. screw  
Titanium Grade 5 ELI



T 100-1

T 105-1

T 110-1

T 120-1

★

### STRAIGHT ABUTMENT

Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



T 100

T 105

T 110

T 120

★

### STRAIGHT MASSIV ABUTMENT

incl. 2 screws  
Titanium Grade 5 ELI



—

T 405

—

—

★

### ABUTMENT SCREW

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



T 60

T 60

T 60

T 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# T-SERIES

compatible to: DENTSPLY Implants® / Xive®



## PLATFORM

3,4 mm

3,8 mm

4,5 mm

## ANGLED ABUTMENT 16°

angled over surface  
Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



T 200-1

T 205-1

T 210-1

## ANGLED ABUTMENT 16°

angled over edge  
Gingiva Height 2,5 mm  
incl. screw  
Titanium Grade 5 ELI



T 200-2

T 205-2

T 210-2

## ANGLED ABUTMENT 16°

angled over surface  
Gingiva Height 1,0 mm  
incl. screw  
Titanium Grade 5 ELI



T 200-1-1

T 205-1-1

T 210-1-1

## ANGLED ABUTMENT 16°

angled over edge  
Gingiva Height 1,0 mm  
incl. screw  
Titanium Grade 5 ELI



T 200-2-1

T 205-2-1

T 210-2-1

## UCLA ABUTMENT

engaging  
incl. screw



—

—

T 11.CA4.500

## ABUTMENT SCREW

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



T 60

T 60


T 60

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# THO-SERIES

compatible to: Thommen Medical® / SPI®

**PLATFORM**




	3,5 mm	4,0 mm	4,5 mm	5,0 mm	6,0 mm
--	--------	--------	--------	--------	--------

**TITANIUM BASE**  
for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



THO 80350000	THO 80400000	THO 80450000	THO 80500000	THO 80600000
--------------	--------------	--------------	--------------	--------------

**SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning




THO 9.S3D3.500	THO 9.S3D4.000	THO 9.S3D4.500	THO 9.S3D5.000	THO 9.S3D6.000	★
----------------	----------------	----------------	----------------	----------------	---

**NT-MILL LAB ANALOG**  
Stainless Steel



THO 5.La3.500	THO 5.La4.000	THO 5.La4.500	THO 5.La5.000	THO 5.La6.000	★
---------------	---------------	---------------	---------------	---------------	---

**IMPLANT PICK-UP**  
for open-tray with  
integrated screw  
**Coming soon**

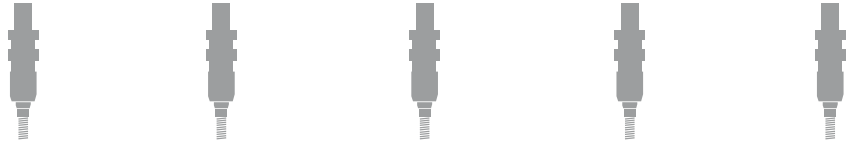

THO TR-00013.5	THO TR-00024.0	THO TR-00034.5	THO TR-00045.0	THO TR-00056.0
----------------	----------------	----------------	----------------	----------------

**ABUTMENT SCREW**  
Recommended tightening  
torques 3,5 mm = 15 Ncm  
4,0 - 6,0 mm = 25 Ncm  
Titanium Grade 5 ELI



THO 603500	THO 604060	THO 604060	THO 604060	THO 604060
------------	------------	------------	------------	------------

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 



# UPR-SERIES

compatible to: Sweden & Martina Implantology™ / Premium Kohno®



**PLATFORM**

3,3 mm

3,8 mm

4,25 mm

5,0 mm

**TITANIUM BASE**

for individual milled Zirconium Abutment incl. screw  
Titanium Grade 5 ELI



UPR 80330000

UPR 80380000

UPR 80420000

UPR 80500000

**SCAN BODY 3D-GUIDE®**

for intra + extra oral scanning



UPR 9.S3D3.300

UPR 9.S3D3.800

UPR 9.S3D4.200

UPR 9.S3D5.000

★

**NT-MILL LAB ANALOG**

Stainless Steel



UPR 5.La3.300

UPR 5.La3.800

UPR 5.La4.200

UPR 5.La5.000

★

**IMPLANT PICK-UP**

for open-tray with integrated screw  
Coming soon



UPR TR-00013.3


UPR TR-00023.8

UPR TR-00034.2

UPR TR-00045.0

**ABUTMENT SCREW**

Recommended tightening torques 25 Ncm  
Titanium Grade 5 ELI



UPR 603338

UPR 603338

UPR 604250

UPR 604250

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 🇺🇸

# UTG-SERIES

compatible to: Sweden & Martina Implantology™ / Premium TG®



**PLATFORM**

3,3 - 4,25 mm

5,0 mm

**TITANIUM BASE**

for individual milled  
Zirconium Abutment  
incl. screw  
Titanium Grade 5 ELI



UTG 80334200

UTG 80500000

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



UTG 9.S3D3.342

UTG 9.S3D5.000

★

**NT-MILL LAB ANALOG**

Stainless Steel



UTG 5.La3.342

UTG 5.La5.000

★

**IMPLANT PICK-UP**

for open-tray with  
integrated screw  
Coming soon



UTG TR-00013.3

UTG TR-00025.0

**ABUTMENT SCREW**

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



UTG 603342

UTG 605000

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# COLOURED MILLING SCREW



The delivered, coloured marked screw, will be used as Milling or Lab Screw for the nt-Preform® Abutment. For all Implant Series and diameters you have to use a Screwdriver with Torx T6. Exception is THO-Serie (Thommen Medical), with a 4-lobe screwdriver.

For the fixing of the Milling Screw (10 Ncm) on un-machined nt-Preform® Abutment, you have to use the long-shaft screwdriver with article-number W 12.WS0.000 and for Thommen W 11.TH0.MIL.

For the fixing of the Milling Screw on finished milled nt-Preform Abutment, can be used from the column Lab-screw.


## USAGE COLOURED MILLING SCREW

SERIES	LAB	MILLING	TORQUE
All Implant Series (except THO-Series)	W 11.LN0.G40 on page 170	W 12.WS0.000 on page 144	10 Ncm
	W 11.LN2.COF on page 172		10 Ncm
THO-Series	W 11.TH0.G04 on page 169	W 11.TH0.MIL on page 144	10 Ncm
	W 11.TH0.000 on page 173		10 Ncm

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with \* are available in the USA 

# 2-CONnect®

ANGLE COMPENSATION FOR DIVERGENT IMPLANTS  
available in different gingiva heights and angled version



## BENEFITS:

- self - centering conical connection
- maximum flexibility of divergent implant positions
- stressless fitting by optional adhesive connection ( female part )
- force application caused by tube shape and integrated screw (Straight Abutment) or mounted screw (Angled Abutment)
- female part compatible between the different implant systems and diameters



## APPLICATION:

- bars
- bridges
- non-engaging structures



## TECHNICAL DETAILS:

- Titanium Grade 5 ELI



## COPING (FEMALE PART) ON 2-CONNECT®

\*Female = glued



## ABUTMENT (MALE PART) ON 2-CONNECT®

\*Male = screwed



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with \* are available in the USA

# TABLE OF CONTENTS

NT CATALOGUE 2017-1

<b>1</b>	<b>TITANIUM BASE ABUTMENT</b>	10 – 49
<b>2</b>	<b>2-CONnect® ABUTMENT</b>	50 – 117
<b>3</b>	<b>NT-PREFORMS® ABUTMENT</b>	118 – 147
<b>4</b>	<b>DIM ANALOG</b>	148 – 161
<b>5</b>	<b>SURGICAL GUIDE SLEEVES</b>	163 – 165
<b>6</b>	<b>TOOLS &amp; DISCS</b>	167 – 181
<b>7</b>	<b>NT-iDent</b>	182 – 189
<b>8</b>	<b>SPECIFICATION</b>	190 – 191

## **BEG-SERIES – NEW**

is compatible to: BEGO Implant Systems® / Semados®  
S, RS-RX, RI-Line - - - - - 52

## **BIO-SERIES – NEW**

is compatible to: BioHorizons® / internal- - - - - 55

## **BRE-SERIES – NEW**

is compatible to: Bredent Medical® / Sky® - - - - - 58

## **CAM-SERIES**

is compatible to: Altatec® / Camlog® - - - - - 61

## **COL-SERIES – NEW**

is compatible to: Altatec® / Conelog® - - - - - 64

## **E-SERIES**

is compatible to: Nobel Biocare™ / Replace Select® - - - - - 67

## **F-SERIES**

is compatible to: Nobel Biocare™ / Nobel Active™ - - - - - 70

## **H-SERIES**

is compatible to: Biomet 3i® / Certain® - - - - - 73

## **HIO-SERIES – NEW**

is compatible to: HIOSSSEN® / OSSTEM TS® - - - - - 76

## **L-SERIES**

is compatible to: Straumann / Bone Level® - - - - - 79

## **MEX-SERIES – NEW**

is compatible to: Medentis Medical® / ICX® - - - - - 82

## **MIC-SERIES – NEW**

is compatible to: MIS® / C1® - - - - - 85

## **MIS-SERIES – NEW**

is compatible to: MIS® / SEVEN® - - - - - 88

## **N-SERIES**

is compatible to: Straumann / SynOcta® - - - - - 91

## **NEO-SERIES – NEW**

is compatible to: NEOSS Implant System® / NEOSS™ - - - - - 94

## **R-SERIES**

is compatible to: Zimmer Dental / Tapered Screw-Vent® - - - 97

## **S-SERIES**

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System OsseoSpeed® TX - - - - - 100

## **SEV-SERIES – NEW**

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System™ EV - - - - - 103

## **T-SERIES**

is compatible to: DENTSPLY Implants® / Xive® - - - - - 106

## **THO-SERIES – NEW**

is compatible to: Thommen Medical® / SPI® - - - - - 109

## **UPR-SERIES – NEW**

is compatible to: Sweden & Martina Implantology™ /  
Premium Kohno® - - - - - 112

## **UTG-SERIES – NEW**

is compatible to: Sweden & Martina Implantology™ /  
Premium TG® - - - - - 115



# BEG-SERIES

compatible to: BEGO Implant Systems® / Semados® S, RS-RX, RI-Line



**PLATFORM**

3,25 / 3,75 mm

4,1 mm

4,5 mm

5,5 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping and Coping-screw  
Titanium Grade 5 ELI

Coming soon



Gingiva Height	0,5 mm	BEG-2CON 8032371S	BEG-2CON 8041001S	BEG-2CON 8045001S	BEG-2CON 8055001S
	2,5 mm	BEG-2CON 8032372S	BEG-2CON 8041002S	BEG-2CON 8045002S	BEG-2CON 8055002S

**2-CONNECT®-ABUTMENT**

Recommended tightening torques: 30 Ncm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



Gingiva Height	0,5 mm	BEG-2CON 8032371M	BEG-2CON 8041001M	BEG-2CON 8045001M	BEG-2CON 8055001M
	2,5 mm	BEG-2CON 8032372M	BEG-2CON 8041002M	BEG-2CON 8045002M	BEG-2CON 8055002M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening torques: 25 Ncm  
Titanium Grade 5 ELI



KS 61

KS 61

KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# BEG-SERIES

compatible to: BEGO Implant Systems® / Semados® S, RS-RX, RI-Line



**PLATFORM**

3,25 / 3,75 mm

4,1 mm

4,5 mm

5,5 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



BEG-2CON 80323A3S

BEG-2CON 80410A3S

BEG-2CON 80450A3S

BEG-2CON 80550A3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



BEG-2CON 80323A3M

BEG-2CON 80410A3M

BEG-2CON 80450A3M

BEG-2CON 80550A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI

Coming soon



BEG 6.Ms3.255

BEG 6.Ms3.255

BEG 6.Ms3.255

BEG 6.Ms3.255

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# BEG-SERIES

compatible to: BEGO Implant Systems® / Semados® S, RS-RX, RI-Line



**PLATFORM**

3,25 / 3,75 mm

4,1 mm

4,5 mm

5,5 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw




● Straight KS 61 = $\varnothing$ 1,8 mm	2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning




● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	★

**2-CONNECT®-  
LAB ANALOG**



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	★

**2-CONNECT®-  
DIM ANALOG**



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	★
---------------	---------------	---------------	---------------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA



# BIO-SERIES

compatible to: BioHorizons® / internal



**PLATFORM**

3,0 mm

3,5 mm

4,5 mm

5,7 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONNECT®-Coping  
and Coping-screw  
Titanium Grade 5 ELI  
Coming soon



Gingiva Height

0,5 mm  
2,5 mm

BIO-2CON 8030001S	BIO-2CON 8035001S	BIO-2CON 8045001S	BIO-2CON 8057001S
BIO-2CON 8030002S	BIO-2CON 8035002S	BIO-2CON 8045002S	BIO-2CON 8057002S

**2-CONNECT®-ABUTMENT**

Recommended tightening  
torques: 30 Ncm  
Titanium Grade 5 ELI  
Coming soon



M (Male Part)

Gingiva Height

0,5 mm  
2,5 mm

BIO-2CON 8030001M	BIO-2CON 8035001M	BIO-2CON 8045001M	BIO-2CON 8057001M
BIO-2CON 8030002M	BIO-2CON 8035002M	BIO-2CON 8045002M	BIO-2CON 8057002M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI

F (Female Part)



2CON F-U	2CON F-U	2CON F-U	2CON F-U	★
----------	----------	----------	----------	---

**COPING-SCREW**

Recommended tightening  
torques: 25 Ncm  
Titanium Grade 5 ELI



KS 61	KS 61	KS 61	KS 61	★
-------	-------	-------	-------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# BIO-SERIES

compatible to: BioHorizons® / internal



**PLATFORM**

3,0 mm

3,5 mm

4,5 mm

5,7 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



BIO-2CON 80300A3S

BIO-2CON 80350A3S

BIO-2CON 80450A3S

BIO-2CON 80570A3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



BIO-2CON 80300A3M

BIO-2CON 80350A3M

BIO-2CON 80450A3M

BIO-2CON 80570A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI

Coming soon



BIO 6.Ms3.057

BIO 6.Ms3.057

BIO 6.Ms3.057

BIO 6.Ms3.057

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# BIO-SERIES

compatible to: BioHorizons® / internal



**PLATFORM**

3,0 mm

3,5 mm

4,5 mm

5,7 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8
2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	★
2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	★

**2-CONNECT®-  
LAB ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	★
2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	★

**2-CONNECT®-  
DIM ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	★
2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	★
---------------	---------------	---------------	---------------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# BRE-SERIES

compatible to: *Bredent Medical® / Sky®*



**PLATFORM**

3,5 mm

4,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Coming soon

Gingiva Height : 0,5 mm  
: 2,5 mm

BRE-2CON 8035001S	BRE-2CON 8040001S
BRE-2CON 8035002S	BRE-2CON 8040002S

**2-CONNECT®-ABUTMENT**

Recommended tightening  
torques: 25 Ncm  
Titanium Grade 5 ELI



Coming soon

M (Male Part)

Gingiva Height : 0,5 mm  
: 2,5 mm

BRE-2CON 8035001M	BRE-2CON 8040001M
BRE-2CON 8035002M	BRE-2CON 8040002M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U	2CON F-U	★
----------	----------	---

**COPING-SCREW**

Recommended tightening  
torques: 20 Ncm  
Titanium Grade 5 ELI



KS 61	KS 61	★
-------	-------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# BRE-SERIES

compatible to: Bredent Medical® / Sky®



**PLATFORM**

3,5 mm

4,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon



BRE-2CON 80350A3S

BRE-2CON 80400A3S

**2-CONNECT®-ABUTMENT**

angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon

M (Male Part)



BRE-2CON 80350A3M

BRE-2CON 80400A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U



**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



BRE 6.Ms3.540

BRE 6.Ms3.540

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 🇺🇸

# BRE-SERIES

compatible to: Bredent Medical® / Sky®



**PLATFORM**

3,5 mm

4,0 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8
2CON TR-00031.6

2CON TR-00021.8
2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800
2CON 9.S3D1.600

2CON 9.S3D1.800
2CON 9.S3D1.600

★  
★

**2-CONNECT®-  
LAB ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800
2CON 5.La1.600

2CON 5.La1.800
2CON 5.La1.600

★  
★

**2-CONNECT®-  
DIM ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180
2CON 5.DIM.160

2CON 5.DIM.180
2CON 5.DIM.160

★  
★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# CAM-SERIES

compatible to: Altatec® / Camlog®



## PLATFORM

3,3 mm

3,8 mm

4,3 mm

5,0 mm

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height : 0,5 mm  
: 2,5 mm

CAM-2CON 8033001S

CAM-2CON 8038001S

CAM-2CON 8043001S

CAM-2CON 8050001S

soon

CAM-2CON 8033002S

CAM-2CON 8038002S

CAM-2CON 8043002S

CAM-2CON 8050002S

## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques:  
Titanium Grade 5 ELI  
M (Male Part)



20 Ncm



30 Ncm



30 Ncm



30 Ncm

Gingiva Height : 0,5 mm  
: 2,5 mm

CAM-2CON 8033001M

CAM-2CON 8038001M

CAM-2CON 8043001M

CAM-2CON 8050001M

soon

CAM-2CON 8033002M

CAM-2CON 8038002M

CAM-2CON 8043002M

CAM-2CON 8050002M

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

2CON F-U

★

## COPING-SCREW

Recommended tightening  
torques:  
Titanium Grade 5 ELI



15 Ncm



25 Ncm



25 Ncm



25 Ncm

KS 61

KS 61

KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# CAM-SERIES

compatible to: Altatec® / Camlog®



## PLATFORM

3,3 mm

3,8 mm

4,3 mm

5,0 mm

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



over edge	CAM-2CON 80330A3S	CAM-2CON 80380A3S	CAM-2CON 80430A3S	CAM-2CON 80500A3S
over surface	CAM-2CON 80330C3S	CAM-2CON 80380C3S	CAM-2CON 80430C3S	CAM-2CON 80500C3S

## 2-CONNECT®-ABUTMENT

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



over edge	CAM-2CON 80330A3M	CAM-2CON 80380A3M	CAM-2CON 80430A3M	CAM-2CON 80500A3M
over surface	CAM-2CON 80330C3M	CAM-2CON 80380C3M	CAM-2CON 80430C3M	CAM-2CON 80500C3M

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U	2CON F-U	2CON F-U	2CON F-U
----------	----------	----------	----------

★

## COPING-SCREW

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI



KS 62	KS 62	KS 62	KS 62
-------	-------	-------	-------

★

## MALE PART SCREW

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI

Coming soon



CAM 6.Ms3.384	CAM 6.Ms3.384	CAM 6.Ms3.384	CAM 6.Ms5.060
---------------	---------------	---------------	---------------

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# CAM-SERIES

compatible to: Altatec® / Camlog®



## PLATFORM

3,3 mm

3,8 mm

4,3 mm

5,0 mm

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON TR-00021.8

2CON TR-00021.8

2CON TR-00021.8

2CON TR-00021.8

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00031.6

2CON TR-00031.6

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 9.S3D1.800

2CON 9.S3D1.800

2CON 9.S3D1.800

2CON 9.S3D1.800

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.600

2CON 9.S3D1.600

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG

Stainless Steel



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 5.La1.800

2CON 5.La1.800

2CON 5.La1.800

2CON 5.La1.800

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.600

2CON 5.La1.600

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 5.DIM.180

2CON 5.DIM.180

2CON 5.DIM.180

2CON 5.DIM.180

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.160

2CON 5.DIM.160

2CON 5.DIM.160

2CON 5.DIM.160

★

## SLEEVE

plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# COL-SERIES

compatible to: Altatec® / Conelog®



## PLATFORM

3,3 mm

3,8 / 4,3 mm

5,0 mm

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONNECT®-Coping and Coping-screw

Titanium Grade 5 ELI

Coming soon



Gingiva Height : 0,5 mm  
: 2,5 mm

COL-2CON 8033001S

COL-2CON 8038431S

COL-2CON 8050001S

COL-2CON 8033002S

COL-2CON 8038432S

COL-2CON 8050002S

## 2-CONNECT®-ABUTMENT

Recommended tightening torques:

Titanium Grade 5 ELI

M (Male Part)



20 Ncm



30 Ncm



30 Ncm

Gingiva Height : 0,5 mm  
: 2,5 mm

COL-2CON 8033001M

COL-2CON 8038431M

COL-2CON 8050001M

COL-2CON 8033002M

COL-2CON 8038432M

COL-2CON 8050002M

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

★

## COPING-SCREW

Recommended tightening torques:

Titanium Grade 5 ELI



15 Ncm



20 Ncm



20 Ncm

KS 61

KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# COL-SERIES

compatible to: Altatec® / Conelog®



**PLATFORM**

3,3 mm

3,8 / 4,3 mm

5,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



over edge	COL-2CON 80330A3S	COL-2CON 80384A3S	COL-2CON 80500A3S
over surface	COL-2CON 80330C3S	COL-2CON 80384C3S	COL-2CON 80500C3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

**M (Male Part)**



over edge	COL-2CON 80330A3M	COL-2CON 80384A3M	COL-2CON 80500A3M
over surface	COL-2CON 80330C3M	COL-2CON 80384C3M	COL-2CON 80500C3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)	2CON F-U	2CON F-U	2CON F-U	★
-----------------	----------	----------	----------	---

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62	KS 62	KS 62
-------	-------	-------

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



COL 6.Ms3.343	COL 6.Ms3.343	COL 6.Ms5.000
---------------	---------------	---------------

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 🇺🇸

# COL-SERIES

compatible to: Altatec® / Conelog®



## PLATFORM

3,3 mm

3,8 / 4,3 mm

5,0 mm

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8

2CON TR-00021.8

2CON TR-00021.8

2CON TR-00031.6

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800

2CON 9.S3D1.800

2CON 9.S3D1.800

★

2CON 9.S3D1.600

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG

Stainless Steel



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800

2CON 5.La1.800

2CON 5.La1.800

★

2CON 5.La1.600

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180

2CON 5.DIM.180

2CON 5.DIM.180

★

2CON 5.DIM.160

2CON 5.DIM.160

2CON 5.DIM.160

★

## SLEEVE

plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# E-SERIES

compatible to: Nobel Biocare™ / Replace Select®



## PLATFORM

3,5 mm NP

4,3 mm RP

5,0 mm WP

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height

0,5 mm

2,5 mm

E 800 S

E 810 S

E 820 S

E-2CON 8035002S

E-2CON 8043002S

E-2CON 8050002S

★

★

## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI  
M (Male Part)



Gingiva Height

0,5 mm

2,5 mm

E 800 M

E 810 M

E 820 M

E-2CON 8035002M

E-2CON 8043002M

E-2CON 8050002M

★

★

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

★

## COPING-SCREW

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



KS 61

KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# E-SERIES

compatible to: Nobel Biocare™ / Replace Select®



**PLATFORM**

3,5 mm NP

4,3 mm RP

5,0 mm WP

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



over edge	E-2CON 80350A3S	E-2CON 80430A3S	E-2CON 80500A3S
over surface	E-2CON 80350C3S	E-2CON 80430C3S	E-2CON 80500C3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

**M (Male Part)**



over edge	E-2CON 80350A3M	E-2CON 80430A3M	E-2CON 80500A3M
over surface	E-2CON 80350C3M	E-2CON 80430C3M	E-2CON 80500C3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)	2CON F-U	2CON F-U	2CON F-U	★
-----------------	----------	----------	----------	---

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI

Coming soon



KS 62	KS 62	KS 62
-------	-------	-------

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI

Coming soon



E 6.Ms3.500	E 6.Ms4.350	E 6.Ms4.350
-------------	-------------	-------------

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# E-SERIES

compatible to: Nobel Biocare™ / Replace Select®



## PLATFORM

3,5 mm NP

4,3 mm RP

5,0 mm WP

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON TR-00021.8

2CON TR-00021.8

2CON TR-00021.8

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00031.6

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 9.S3D1.800

2CON 9.S3D1.800

2CON 9.S3D1.800

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.600

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG

Stainless Steel



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 5.La1.800

2CON 5.La1.800

2CON 5.La1.800

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.600

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 5.DIM.180

2CON 5.DIM.180

2CON 5.DIM.180

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.160

2CON 5.DIM.160

2CON 5.DIM.160

★

## SLEEVE

plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# F-SERIES

compatible to: Nobel Biocare™ / Nobel Active™



## PLATFORM

3,5 mm NP

4,3 / 5,0 mm RP

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height	0,5 mm	F 800 S	F 810 S	★
	2,5 mm	F-2CON 8035002S	F-2CON 8043002S	★

## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques: NP = 25 Ncm  
RP = 35 Ncm  
Titanium Grade 5 ELI



M (Male Part)

Gingiva Height	0,5 mm	F 800 M	F 810 M	★
	2,5 mm	F-2CON 8035002M	F-2CON 8043002M	★

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U	2CON F-U	★
----------	----------	---

## COPING-SCREW

Recommended tightening  
torques:  
Titanium Grade 5 ELI



KS 61	KS 61	★
-------	-------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# F-SERIES

compatible to: Nobel Biocare™ / Nobel Active™



**PLATFORM**

3,5 mm NP

4,3 / 5,0 mm RP

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20° Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



F-2CON 80350A3S

F-2CON 80430A3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

**M (Male Part)**

Coming soon



F-2CON 80350A3M

F-2CON 80430A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI

**F (Female Part)**



2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI

Coming soon



F 6.Ms3.500

F 6.Ms4.350

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# F-SERIES

compatible to: Nobel Biocare™ / Nobel Active™



## PLATFORM

3,5 mm NP

4,3 / 5,0 mm RP

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON TR-00021.8

2CON TR-00021.8

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 9.S3D1.800

2CON 9.S3D1.800

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG

Stainless Steel



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 5.La1.800

2CON 5.La1.800

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 5.DIM.180

2CON 5.DIM.180

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.160

2CON 5.DIM.160

★

## SLEEVE

plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# H-SERIES

compatible to: Biomet 3i® / Certain®



## PLATFORM

3,4 mm NP

4,1 mm RP

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONNECT®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height	0,5 mm	H 800 S	H 810 S	★
	2,5 mm	H-2CON 8034002S	H-2CON 8041002S	★

## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques 20 Ncm  
Titanium Grade 5 ELI

**M** (Male Part)



Gingiva Height	0,5 mm	H 800 M	H 810 M	★
	2,5 mm	H-2CON 8034002M	H-2CON 8041002M	★

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)	2CON F-U	2CON F-U	★
-----------------	----------	----------	---

## COPING-SCREW

Recommended tightening  
torques 15 Ncm  
Titanium Grade 5 ELI



KS 60	KS 60	★
-------	-------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# H-SERIES

compatible to: Biomet 3i® / Certain®



**PLATFORM**

3,4 mm NP

4,1 mm RP

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI  
**Coming soon**



H-2CON 80340A3S

H-2CON 80410A3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI  
**Coming soon**  
**M (Male Part)**



H-2CON 80410A3M

H-2CON 80410A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



**F (Female Part)**

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques 15 Ncm  
Titanium Grade 5 ELI  
**Coming soon**



KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI  
**Coming soon**



H 6.Ms3.450

H 6.Ms3.450

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# H-SERIES

compatible to: Biomet 3i® / Certain®



## PLATFORM

3,4 mm NP

4,1 mm RP

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



● Straight KS 60 =  $\varnothing$  1,4 mm

2CON TR-00011.4

2CON TR-00011.4

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



● Straight KS 60 =  $\varnothing$  1,4 mm

2CON 9.S3D1.400

2CON 9.S3D1.400

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG

Stainless Steel



● Straight KS 60 =  $\varnothing$  1,4 mm

2CON 5.La1.400

2CON 5.La1.400

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



● Straight KS 60 =  $\varnothing$  1,4 mm

2CON 5.DIM.140

2CON 5.DIM.140

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.160

2CON 5.DIM.160

★

## SLEEVE

plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# HIO-SERIES

compatible to: HIOSSEN® / OSSTEM TS®



**PLATFORM**

3,5 mm

4,0 - 6,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI

Coming soon



Gingiva Height	0,5 mm	HIO-2CON 8035001S	HIO-2CON 8040601S
	2,5 mm	HIO-2CON 8035002S	HIO-2CON 8040602S

**2-CONNECT®-ABUTMENT**

Recommended tightening  
torques: 3,5 mm = 20 Ncm  
4,0 - 6,0 mm = 30 Ncm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



Gingiva Height	0,5 mm	HIO-2CON 8035001M	HIO-2CON 8040601M
	2,5 mm	HIO-2CON 8035002M	HIO-2CON 8040602M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)	2CON F-U	2CON F-U	★
-----------------	----------	----------	---

**COPING-SCREW**

Recommended tightening  
torques:  
Titanium Grade 5 ELI



	KS 61	KS 61	★
--	-------	-------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# HIO-SERIES

compatible to: HIOSSEN® / OSSTEM TS®



**PLATFORM**

3,5 mm

4,0 - 6,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI



Coming soon

HIO-2CON 80350A3S

HIO-2CON 80406A3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI



Coming soon

M (Male Part)

HIO-2CON 80350A3M

HIO-2CON 80406A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI



Coming soon

KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI



Coming soon

HIO 6.Ms3.500

HIO 6.Ms4.060

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 🇺🇸

# HIO-SERIES

compatible to: HIOSSEN® / OSSTEM TS®



**PLATFORM**

3,5 mm

4,0 - 6,0 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8

2CON TR-00021.8

2CON TR-00031.6

2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800

2CON 9.S3D1.800

2CON 9.S3D1.600

2CON 9.S3D1.600

★

★

**2-CONNECT®-  
LAB ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800

2CON 5.La1.800

2CON 5.La1.600

2CON 5.La1.600

★

★

**2-CONNECT®-  
DIM ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180

2CON 5.DIM.180

2CON 5.DIM.160

2CON 5.DIM.160

★

★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# L-SERIES

compatible to: Straumann / Bone Level®



## PLATFORM

3,3 mm NC

4,1 / 4,8 mm RC

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height : 0,5 mm  
: 2,5 mm

L 800 S

L 810 S



L-2CON 8033002S

L-2CON 8041482S



## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI  
M (Male Part)



Gingiva Height : 0,5 mm  
: 2,5 mm

L 800 M

L 810 M



L-2CON 8033002M

L-2CON 8041482M



## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U



## COPING-SCREW

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



KS 61

KS 61



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# L-SERIES

compatible to: Straumann / Bone Level®



**PLATFORM**

3,3 mm NC

4,1 / 4,8 mm RC

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



over surface	L-2CON 80330A3S	L-2CON 84148A3S
over edge	L-2CON 80330C3S	L-2CON 84148C3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



over surface	L-2CON 80330A3M	L-2CON 84148A3M
over edge	L-2CON 80330C3M	L-2CON 84148C3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)	2CON F-U	2CON F-U	★
-----------------	----------	----------	---

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI

Coming soon



KS 62	KS 62
-------	-------

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI

Coming soon



L 6.Ms3.341	L 6.Ms3.341
-------------	-------------

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# L-SERIES

compatible to: Straumann / Bone Level®



## PLATFORM

3,3 mm NC

4,1 / 4,8 mm RC

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8

2CON TR-00021.8

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800

2CON 9.S3D1.800

★

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG

Stainless Steel



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800

2CON 5.La1.800

★

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180

2CON 5.DIM.180

★

2CON 5.DIM.160

2CON 5.DIM.160

## SLEEVE

plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# MEX-SERIES

compatible to: Medentis Medical® / ICX®



**PLATFORM**

3,45 - 4,8 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height	0,5 mm	MEX-2CON 8041481S
	2,5 mm	MEX-2CON 8041482S

**2-CONNECT®-ABUTMENT**

Recommended tightening  
torques: 30 Ncm  
Titanium Grade 5 ELI  
**M** (Male Part)



Gingiva Height	0,5 mm	MEX-2CON 8041481M
	2,5 mm	MEX-2CON 8041482M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)	2CON F-U	★
-----------------	----------	---

**COPING-SCREW**

Recommended tightening  
torques: 25 Ncm  
Titanium Grade 5 ELI



KS 61	★
-------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# MEX-SERIES

compatible to: Medentis Medical® / ICX®



## PLATFORM

3,45 - 4,8 mm

### 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon



MEX-2CON 80414A3S

### 2-CONNECT®-ABUTMENT

angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon

M (Male Part)



MEX-2CON 80414A3M

### 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U



### COPING-SCREW

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

### MALE PART SCREW

for angled 20° 2-CONnect®

Abutment | Recommended

tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



MEX 6.Ms4.148

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# MEX-SERIES

compatible to: Medentis Medical® / ICX®



**PLATFORM**

3,45 - 4,8 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm      2CON TR-00021.8
- Angled KS 62 =  $\varnothing$  1,6 mm      2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm      2CON 9.S3D1.800      ★
- Angled KS 62 =  $\varnothing$  1,6 mm      2CON 9.S3D1.600      ★

**2-CONNECT®-  
LAB ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm      2CON 5.La1.800      ★
- Angled KS 62 =  $\varnothing$  1,6 mm      2CON 5.La1.600      ★

**2-CONNECT®-  
DIM ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm      2CON 5.DIM.180      ★
- Angled KS 62 =  $\varnothing$  1,6 mm      2CON 5.DIM.160      ★

**SLEEVE**  
for plaster model  
Stainless Steel



- DIM 5.XSL.A30      ★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# MIC-SERIES

compatible to: MIS® / C1®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height : 0,5 mm  
: 2,5 mm

MIC-2CON 8033001S

MIC-2CON 8037421S

MIC-2CON 8050001S

MIC-2CON 8033002S

MIC-2CON 8037422S

MIC-2CON 8050002S **soon**

**2-CONNECT®-ABUTMENT**

Recommended tightening  
torques: 30 Ncm  
Titanium Grade 5 ELI  
**M** (Male Part)



Gingiva Height : 0,5 mm  
: 2,5 mm

MIC-2CON 8033001M

MIC-2CON 8037421M

MIC-2CON 8050001M

MIC-2CON 8033002M

MIC-2CON 8037422M

MIC-2CON 8050002M **soon**

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 25 Ncm  
Titanium Grade 5 ELI



KS 61

KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# MIC-SERIES

compatible to: MIS® / C1®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



over edge

MIC-2CON 80330A3S

MIC-2CON 80374A3S

MIC-2CON 80500A3S

over surface

MIC-2CON 80330A3S

—

—

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

**M (Male Part)**

Coming soon



over edge

MIC-2CON 80330A3M

MIC-2CON 80374A3M

MIC-2CON 80500A3M

over surface

MIC-2CON 80330A3M

—

—

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



MIC 6.Ms3.300

MIC 6.Ms3.750

MIC 6.Ms3.750

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# MIC-SERIES

compatible to: MIS® / C1®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8
2CON TR-00031.6

2CON TR-00021.8
2CON TR-00031.6

2CON TR-00021.8
2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800
2CON 9.S3D1.600

2CON 9.S3D1.800
2CON 9.S3D1.600

2CON 9.S3D1.800
2CON 9.S3D1.600

★  
★

**2-CONNECT®-  
LAB ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800
2CON 5.La1.600

2CON 5.La1.800
2CON 5.La1.600

2CON 5.La1.800
2CON 5.La1.600

★  
★

**2-CONNECT®-  
DIM ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180
2CON 5.DIM.160

2CON 5.DIM.180
2CON 5.DIM.160

2CON 5.DIM.180
2CON 5.DIM.160

★  
★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# MIS-SERIES

compatible to: MIS® / SEVEN®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height : 0,5 mm  
: 2,5 mm

MIS-2CON 8033001S

MIS-2CON 8037421S

MIS-2CON 8050001S

MIS-2CON 8033002S

MIS-2CON 8037422S

MIS-2CON 8050002S **soon**

**2-CONNECT®-ABUTMENT**

Recommended tightening  
torques: 30 Ncm  
Titanium Grade 5 ELI  
**M (Male Part)**



Gingiva Height : 0,5 mm  
: 2,5 mm

MIS-2CON 8033001M

MIS-2CON 8037421M

MIS-2CON 8050001M

MIS-2CON 8033002M

MIS-2CON 8037422M

MIS-2CON 8050002M **soon**

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



**F (Female Part)**

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 25 Ncm  
Titanium Grade 5 ELI



KS 61

KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# MIS-SERIES

compatible to: MIS® / SEVEN®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI  
**Coming soon**



MIS-2CON 8033002S

MIS-2CON 8037422S

MIS-2CON 8050002S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI  
**Coming soon**  
**M (Male Part)**



MIS-2CON 8033002M

MIS-2CON 8037422M

MIS-2CON 8050002M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



**F (Female Part)**

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI  
**Coming soon**



KS 62

KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI  
**Coming soon**



MIS 6.Ms3.300

MIS 6.MS3.750

MIS 6.MS3.750

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 🇺🇸

# MIS-SERIES

compatible to: MIS® / SEVEN®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8
2CON TR-00031.6

2CON TR-00021.8
2CON TR-00031.6

2CON TR-00021.8
2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800
2CON 9.S3D1.600

2CON 9.S3D1.800
2CON 9.S3D1.600

2CON 9.S3D1.800
2CON 9.S3D1.600

★  
★

**2-CONNECT®-  
LAB ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800
2CON 5.La1.600

2CON 5.La1.800
2CON 5.La1.600

2CON 5.La1.800
2CON 5.La1.600

★  
★

**2-CONNECT®-  
DIM ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180
2CON 5.DIM.160

2CON 5.DIM.180
2CON 5.DIM.160

2CON 5.DIM.180
2CON 5.DIM.160

★  
★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30
---------------

DIM 5.XSL.A30
---------------

DIM 5.XSL.A30
---------------

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# N-SERIES

compatible to: Straumann / SynOcta®



## PLATFORM

4,8 mm RN

6,5 mm WN

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height

0,5 mm	
2,5 mm	

N 810 S

N 820 S

N-2CON 8048002S

N-2CON 8065002S

★

★

## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI  
M (Male Part)



Gingiva Height

0,5 mm	
2,5 mm	

N 810 M

N 820 M

N-2CON 8048002M

N-2CON 8065002M

★

★

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

★

## COPING-SCREW

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# N-SERIES

compatible to: Straumann / SynOcta®



**PLATFORM**

4,8 mm RN

6,5 mm WN

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon



N-2CON 80480A3S

N-2CON 80650A3M

**2-CONNECT®-ABUTMENT**

angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon

**M** (Male Part)



N-2CON 80480A3M

N-2CON 80650A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



**F** (Female Part)

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



N 6.Ms4.865

N 6.Ms4.865

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# N-SERIES

compatible to: Straumann / SynOcta®



## PLATFORM

4,8 mm RN

6,5 mm WN

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8

2CON TR-00021.8

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800

2CON 9.S3D1.800

★

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG



- GH 0,5 mm - Straight KS 61 =  $\varnothing$  1,8 mm
- GH 2,5 mm - Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800

2CON 5.La6.500.05

★

2CON 5.La6.500

★

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



- GH 0,5 mm - Straight KS 61 =  $\varnothing$  1,8 mm
- GH 2,5 mm - Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180

2CON 5.DIM.650.05

★

2CON 5.DIM.650

★

2CON 5.DIM.160

2CON 5.DIM.160

★

## SLEEVE

for plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# NEO-SERIES

compatible to: *NEOSS Implant System*<sup>®</sup> / *NEOSS*<sup>™</sup>



**PLATFORM**

3,5 - 5,5 mm

**2-CONNECT<sup>®</sup>-ABUTMENT SET**

incl. 2-CONnect<sup>®</sup>-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height	0,5 mm	NEO-2CON 8035551S
	2,5 mm	NEO-2CON 8035552S

**2-CONNECT<sup>®</sup>-ABUTMENT**

Recommended tightening  
torques: 30 Ncm  
Titanium Grade 5 ELI  
**M (Male Part)**



Gingiva Height	0,5 mm	NEO-2CON 8035551M
	2,5 mm	NEO-2CON 8035552M

**2-CONNECT<sup>®</sup>-COPING**

Titanium Grade 5 ELI



**F (Female Part)**

2CON F-U	★
----------	---

**COPING-SCREW**

Recommended tightening  
torques: 25 Ncm  
Titanium Grade 5 ELI




KS 61	★
-------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# NEO-SERIES

compatible to: *NEOSS Implant System® / NEOSS™*



## PLATFORM

3,5 - 5,5 mm

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon



NEO-2CON 80355A3S

## 2-CONNECT®-ABUTMENT

angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon

M (Male Part)



NEO-2CON 80355A3M

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U



## COPING-SCREW

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

## MALE PART SCREW

for angled 20° 2-CONnect®

Abutment | Recommended tightening  
torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



NEO 6.Ms3.555

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# NEO-SERIES

compatible to: *NEOSS Implant System*<sup>®</sup> / *NEOSS*<sup>™</sup>



**PLATFORM**

3,5 - 5,5 mm

**2-CONNECT<sup>®</sup>-  
IMPLANT PICK-UP**  
integrated screw



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON TR-00021.8
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON TR-00031.6

**2-CONNECT<sup>®</sup>-  
SCAN BODY 3D-GUIDE<sup>®</sup>**  
for intra + extra  
oral scanning



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 9.S3D1.800	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 9.S3D1.600	★

**2-CONNECT<sup>®</sup>-  
LAB ANALOG**



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 5.La1.800	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 5.La1.600	★

**2-CONNECT<sup>®</sup>-  
DIM ANALOG**



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 5.DIM.180	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 5.DIM.160	★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30	★
---------------	---

Notice: Products indicated with <sup>®</sup> and <sup>™</sup> are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# R-SERIES

compatible to: Zimmer Dental / Tapered Screw-Vent®



## PLATFORM

3,5 mm

4,5 mm

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height : 0,5 mm  
: 2,5 mm

R 800 S

R 810 S

★

R-2CON 8035002S

R-2CON 8045002S

★

## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI

**M** (Male Part)



Gingiva Height : 0,5 mm  
: 2,5 mm

R 800 M

R 810 M

★

R-2CON 8035002M

R-2CON 8045002M

★

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



**F** (Female Part)

2CON F-U

2CON F-U

★

## COPING-SCREW

Recommended tightening  
torques 15 Ncm  
Titanium Grade 5 ELI



KS 60

KS 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# R-SERIES

compatible to: Zimmer Dental / Tapered Screw-Vent®



**PLATFORM**

3,5 mm

4,5 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



R-2CON 80350A3S

R-2CON 80450A3S

**2-CONNECT®-ABUTMENT**

angled 20°

Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



R-2CON 80350A3M

R-2CON 80450A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torque: 20 Ncm

Titanium Grade 5 ELI

Coming soon



R 6.Ms3.557

R 6.Ms3.557

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# R-SERIES

compatible to: Zimmer Dental / Tapered Screw-Vent®



## PLATFORM

3,5 mm

4,5 mm

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



● Straight KS 60 =  $\varnothing$  1,4 mm

2CON TR-00011.4

2CON TR-00011.4

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



● Straight KS 60 =  $\varnothing$  1,4 mm

2CON 9.S3D1.400

2CON 9.S3D1.400

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG

Stainless Steel



● Straight KS 60 =  $\varnothing$  1,4 mm

2CON 5.La1.400

2CON 5.La1.400

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



● Straight KS 60 =  $\varnothing$  1,4 mm

2CON 5.DIM.140

2CON 5.DIM.140

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.160

2CON 5.DIM.160

★

## SLEEVE

plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# S-SERIES

compatible to: DENTSPLY Implants® / Astra Tech Implant System OsseoSpeed® TX



## PLATFORM

3,5 / 4,0 mm

4,5 / 5,0 mm

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height

0,5 mm

S 800 S

S 820 S

★

2,5 mm

S-2CON 8035402S

S-2CON 8045502S

★

## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI  
M (Male Part)



Gingiva Height

0,5 mm

S 800 M

S 820 M

★

2,5 mm

S-2CON 8035402M

S-2CON 8045502M

★

## 2-CONNECT®-COPING

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

★

## COPING-SCREW

Recommended tightening  
torques 20 Ncm  
Titanium Grade 5 ELI



KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# S-SERIES

compatible to: DENTSPLY Implants® / Astra Tech Implant System OsseoSpeed® TX



**PLATFORM**

3,5 / 4,0 mm

4,5 / 5,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon



S-2CON 80354A3S

S-2CON 80455A3S

**2-CONNECT®-ABUTMENT**

angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon

M (Male Part)



S-2CON 80354A3M

S-2CON 80455A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



S 6.Ms3.540

S 6.Ms4.550

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# S-SERIES

compatible to: DENTSPLY Implants® / Astra Tech Implant System Osseospeed® TX



## PLATFORM

3,5 / 4,0 mm

4,5 / 5,0 mm

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON TR-00021.8

2CON TR-00021.8

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00031.6

2CON TR-00031.6

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 9.S3D1.800

2CON 9.S3D1.800

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.600

2CON 9.S3D1.600

★

## 2-CONNECT®- LAB ANALOG

Stainless Steel



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 5.La1.800

2CON 5.La1.800

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.600

2CON 5.La1.600

★

## 2-CONNECT®- DIM ANALOG



● Straight KS 61 =  $\varnothing$  1,8 mm

2CON 5.DIM.180

2CON 5.DIM.180

★

● Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.160

2CON 5.DIM.160

★

## SLEEVE

plaster model  
Stainless Steel



DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# SEV-SERIE

compatible to: DENTSPLY Implants® / Astra Tech Implant System™ EV



**PLATFORM**

3,0 mm

3,6 mm

4,2 mm

4,8 mm

5,4 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI

\*Coming soon



Gingiva Height	0,5 mm	SEV-2CON 8030001S	SEV-2CON 8036001S	SEV-2CON 8042001S	SEV-2CON 8048001S	SEV-2CON 8054001S
	2,5 mm	SEV-2CON 8030002S	SEV-2CON 8036002S	SEV-2CON 8042002S	SEV-2CON 8048002S*	SEV-2CON 8054002S

**2-CONNECT®-ABUTMENT**

Recommended tightening  
torques: 25 Ncm  
Titanium Grade 5 ELI

\*Coming soon

**M (Male Part)**



Gingiva Height	0,5 mm	SEV-2CON 8030001M	SEV-2CON 8036001M	SEV-2CON 8042001M	SEV-2CON 8048001M	SEV-2CON 8054001M
	2,5 mm	SEV-2CON 8030002M	SEV-2CON 8036002M	SEV-2CON 8042002M	SEV-2CON 8048002M*	SEV-2CON 8054002M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



<b>F (Female Part)</b>	2CON F-U	2CON F-U	2CON F-U	2CON F-U	2CON F-U	★
------------------------	----------	----------	----------	----------	----------	---

**COPING-SCREW**

Recommended tightening  
torques: 20 Ncm  
Titanium Grade 5 ELI



KS 61	KS 61	KS 61	KS 61	KS 61	★
-------	-------	-------	-------	-------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# SEV-SERIE

compatible to: DENTSPLY Implants® / Astra Tech Implant System™ EV



**PLATFORM**

3,0 mm

3,6 mm

4,2 mm

4,8 mm

5,4 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



SEV-2CON 80300A3S

SEV-2CON 80360A3S

SEV-2CON 80420A3S

SEV-2CON 80480A3S

SEV-2CON 80540A3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



SEV-2CON 80300A3M

SEV-2CON 80360A3M

SEV-2CON 80420A3M

SEV-2CON 80480A3M

SEV-2CON 80540A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

KS 62

KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI

Coming soon



SEV 6.Ms3.000

SEV 6.Ms3.600

SEV 6.Ms4.200

SEV 6.Ms4.800

SEV 6.Ms5.400

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# SEV-SERIE

compatible to: DENTSPLY Implants® / Astra Tech Implant System™ EV



**PLATFORM**

3,0 mm

3,6 mm

4,2 mm

4,8 mm

5,4 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	★

**2-CONNECT®-  
LAB ANALOG**



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	★

**2-CONNECT®-  
DIM ANALOG**



● Straight KS 61 = $\varnothing$ 1,8 mm	2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	★
---------------	---------------	---------------	---------------	---------------	---------------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# T-SERIES

compatible to: DENTSPLY Implants® / Xive®



## PLATFORM

3,4 mm

3,8 mm

4,5 mm

## 2-CONNECT®-ABUTMENT SET

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI



Gingiva Height : 0,5 mm  
: 2,5 mm

T 800 S

T 805 S

T 810 S

★

T-2CON 8034002S

T-2CON 8038002S

T-2CON 8045002S

★

## 2-CONNECT®-ABUTMENT

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI  
M (Male Part)



Gingiva Height : 0,5 mm  
: 2,5 mm

T 800 M

T 805 M

T 810 M

★

T-2CON 8034002M

T-2CON 8038002M

T-2CON 8045002M

★

## 2-CONNECT®-COPING

Titanium Grade 5 ELI

F (Female Part)



2CON F-U

2CON F-U

2CON F-U

★

## COPING-SCREW

Recommended tightening  
torques:  
Titanium Grade 5 ELI



15 Ncm

20 Ncm

20 Ncm

KS 60

KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# T-SERIES

compatible to: DENTSPLY Implants® / Xive®



**PLATFORM**

3,4 mm

3,8 mm

4,5 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon



T-2CON 80340A3S

T-2CON 80380A3S

T-2CON 80450A3S

**2-CONNECT®-ABUTMENT**

angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon

M (Male Part)



T-2CON 80340A3M

T-2CON 80380A3M

T-2CON 80450A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



T 6.Ms3.455

T 6.Ms3.455

T 6.Ms3.455

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# T-SERIES

compatible to: DENTSPLY Implants® / Xive®



**PLATFORM**

3,4 mm

3,8 mm

4,5 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



- Straight KS 60 =  $\varnothing$  1,4 mm
- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00011.4	—	—
—	2CON TR-00021.8	2CON TR-00021.8
2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



- Straight KS 60 =  $\varnothing$  1,4 mm
- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.400	—	—	★
—	2CON 9.S3D1.800	CON 9.S3D1.800	★
2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	★

**2-CONNECT®-  
LAB ANALOG**



- Straight KS 60 =  $\varnothing$  1,4 mm
- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.400	—	—	★
—	2CON 5.La1.800	2CON 5.La1.800	★
2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	★

**2-CONNECT®-  
DIM ANALOG**



- Straight KS 60 =  $\varnothing$  1,4 mm
- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.140	—	—	★
—	2CON 5.DIM.180	2CON 5.DIM.180	★
2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	★
---------------	---------------	---------------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# THO-SERIES

compatible to: Thommen Medical® / SPI®



**PLATFORM**

3,5 mm

4,0 mm

4,5 mm

5,0 mm

6,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping

and Coping-screw

Titanium Grade 5 ELI

Coming soon



Gingiva Height : 0,5 mm  
: 2,5 mm

THO-2CON 8035001S	THO-2CON 8040001S	THO-2CON 8045001S	THO-2CON 8050001S	THO-2CON 8060001S
THO-2CON 8035002S	THO-2CON 8040002S	THO-2CON 8045002S	THO-2CON 8050002S	THO-2CON 8060002S

**2-CONNECT®-ABUTMENT**

Recommended tightening

torques: 3,5 mm = 15 Ncm

4,0 - 6,0 mm = 25 Ncm

Titanium Grade 5 ELI

Coming soon

M (Male Part)



Gingiva Height : 0,5 mm  
: 2,5 mm

THO-2CON 8035001M	THO-2CON 8040001M	THO-2CON 8045001M	THO-2CON 8050001M	THO-2CON 8060001M
THO-2CON 8035002M	THO-2CON 8040002M	THO-2CON 8045002M	THO-2CON 8050002M	THO-2CON 8060002M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI

F (Female Part)



2CON F-U	2CON F-U	2CON F-U	2CON F-U	2CON F-U
----------	----------	----------	----------	----------

★

**COPING-SCREW**

Recommended tightening

torques: 3,5 - 4,0 mm = 15 Ncm

4,5 - 6,0 mm = 20 Ncm

Titanium Grade 5 ELI



KS 60	KS 60	KS 61	KS 61	KS 61
-------	-------	-------	-------	-------

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# THO-SERIES

compatible to: Thommen Medical® / SPI®



**PLATFORM**

3,5 mm

4,0 mm

4,5 mm

5,0 mm

6,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon



THO-2CON 80350A3S THO-2CON 80400A3S THO-2CON 80450A3S THO-2CON 80500A3S THO-2CON 80600A3S

**2-CONNECT®-ABUTMENT**

angled 20°  
Gingiva Height 2,5 mm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



THO-2CON 80350A3M THO-2CON 80400A3M THO-2CON 80450A3M THO-2CON 80500A3M THO-2CON 80600A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U 2CON F-U 2CON F-U 2CON F-U 2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm  
Titanium Grade 5 ELI

Coming soon



KS 62 KS 62 KS 62 KS 62 KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm  
Titanium Grade 5 ELI

Coming soon



THO 6.Ms3.500 THO 6.Ms4.060 THO 6.Ms4.060 THO 6.Ms4.060 THO 6.Ms4.060

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# THO-SERIES

compatible to: Thommen Medical® / SPI®



**PLATFORM**

3,5 mm

4,0 mm

4,5 mm

5,0 mm

6,0 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



● Straight KS 60 = $\varnothing$ 1,4 mm	2CON 9.S3D1.400	2CON 9.S3D1.400	—	—	—
● Straight KS 61 = $\varnothing$ 1,8 mm	—	—	2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



● Straight KS 60 = $\varnothing$ 1,4 mm	2CON 9.S3D1.400	2CON 9.S3D1.400	—	—	—	★
● Straight KS 61 = $\varnothing$ 1,8 mm	—	—	2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	★

**2-CONNECT®-  
LAB ANALOG**



● Straight KS 60 = $\varnothing$ 1,4 mm	2CON 5.La1.400	2CON 5.La1.400	—	—	—	★
● Straight KS 61 = $\varnothing$ 1,8 mm	—	—	2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	★

**2-CONNECT®-  
DIM ANALOG**



● Straight KS 60 = $\varnothing$ 1,4 mm	2CON 5.DIM.140	2CON 5.DIM.140	—	—	—	★
● Straight KS 61 = $\varnothing$ 1,8 mm	—	—	2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	★
● Angled KS 62 = $\varnothing$ 1,6 mm	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	★
---------------	---------------	---------------	---------------	---------------	---------------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufacturers. Products indicated with ★ are available in the USA 🇺🇸

# UPR-SERIES

compatible to: Sweden & Martina Implantology™ / Premium Kohno®



**PLATFORM**

3,3 mm

3,8 mm

4,25 mm

5,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping and Coping-screw  
Titanium Grade 5 ELI  
Coming soon



Gingiva Height	0,5 mm	UPR-2CON 8033001S	UPR-2CON 8038001S	UPR-2CON 8042001S	UPR-2CON 8050001S
	2,5 mm	UPR-2CON 8033002S	UPR-2CON 8038002S	UPR-2CON 8042002S	UPR-2CON 8050002S

**2-CONNECT®-ABUTMENT**

Recommended tightening torques: 25 Ncm  
Titanium Grade 5 ELI  
Coming soon  
M (Male Part)



Gingiva Height	0,5 mm	UPR-2CON 8033001M	UPR-2CON 8038001M	UPR-2CON 8042001M	UPR-2CON 8050001M
	2,5 mm	UPR-2CON 8033002M	UPR-2CON 8038002M	UPR-2CON 8042002M	UPR-2CON 8050002M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)	2CON F-U	2CON F-U	2CON F-U	2CON F-U	★
-----------------	----------	----------	----------	----------	---

**COPING-SCREW**

Recommended tightening torques: 20 Ncm  
Titanium Grade 5 ELI



KS 61	KS 61	KS 61	KS 61
-------	-------	-------	-------

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# UPR-SERIES

compatible to: Sweden & Martina Implantology™ / Premium Kohno®



**PLATFORM**

3,3 mm

3,8 mm

4,25 mm

5,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon



UPR-2CON 80330A3S

UPR-2CON 80380A3S

UPR-2CON 80420A3S

UPR-2CON 80500A3S

**2-CONNECT®-ABUTMENT**

angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon

M (Male Part)



UPR-2CON 80330A3M

UPR-2CON 80380A3M

UPR-2CON 80420A3M

UPR-2CON 80500A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI

F (Female Part)



2CON F-U

2CON F-U

2CON F-U

2CON F-U


★

**COPING-SCREW**

Recommended tightening  
torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®  
Abutment | Recommended  
tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



UPR 6.Ms.3.338

UPR 6.Ms.3.338

UPR 6.Ms4.250

UPR 6.Ms4.250

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# UPR-SERIES

compatible to: Sweden & Martina Implantology™ / Premium Kohno®



**PLATFORM**

3,3 mm

3,8 mm

4,25 mm

5,0 mm

**2-CONNECT®-  
IMPLANT PICK-UP**  
integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8	2CON TR-00021.8
2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6	2CON TR-00031.6

**2-CONNECT®-  
SCAN BODY 3D-GUIDE®**  
for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	2CON 9.S3D1.800	★
2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	2CON 9.S3D1.600	★

**2-CONNECT®-  
LAB ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	2CON 5.La1.800	★
2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	2CON 5.La1.600	★

**2-CONNECT®-  
DIM ANALOG**



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	2CON 5.DIM.180	★
2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	2CON 5.DIM.160	★

**SLEEVE**  
for plaster model  
Stainless Steel



DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	DIM 5.XSL.A30	★
---------------	---------------	---------------	---------------	---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# UTG-SERIES

compatible to: Sweden & Martina Implantology™ / Premium TG®



**PLATFORM**

3,3 - 4,25 mm

5,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping  
and Coping-screw  
Titanium Grade 5 ELI

Coming soon



Gingiva Height : 0,5 mm  
                          : 2,5 mm

UTG-2CON 8033421S

UTG-2CON 8050001S

UTG-2CON 8033422S

UTG-2CON 8050002S

**2-CONNECT®-ABUTMENT**

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI

Coming soon

M (Male Part)



Gingiva Height : 0,5 mm  
                          : 2,5 mm

UTG-2CON 8033421M

UTG-2CON 8050001M

UTG-2CON 8033422M

UTG-2CON 8050002M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening  
torques: 20 Ncm  
Titanium Grade 5 ELI



KS 61

KS 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# UTG-SERIES

compatible to: Sweden & Martina Implantology™ / Premium TG®



**PLATFORM**

3,3 - 4,25 mm

5,0 mm

**2-CONNECT®-ABUTMENT SET**

incl. 2-CONnect®-Coping,  
Coping-screw & Male Part Screw  
angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon



UTG-2CON 80334A3S

UTG-2CON 80500A3S

**2-CONNECT®-ABUTMENT**

angled 20°

Gingiva Height 2,5 mm

Titanium Grade 5 ELI

Coming soon

M (Male Part)



UTG-2CON 80334A3M

UTG-2CON 80500A3M

**2-CONNECT®-COPING**

Titanium Grade 5 ELI



F (Female Part)

2CON F-U

2CON F-U

★

**COPING-SCREW**

Recommended tightening

torques: 15 Ncm

Titanium Grade 5 ELI

Coming soon



KS 62

KS 62

**MALE PART SCREW**

for angled 20° 2-CONnect®

Abutment | Recommended

tightening torques: 20 Ncm

Titanium Grade 5 ELI

Coming soon



UTG 6.Ms3.342

UTG 6.Ms5.000

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# UTG-SERIES

compatible to: Sweden & Martina Implantology™ / Premium TG®



## PLATFORM

3,3 - 4,25 mm

5,0 mm

## 2-CONNECT®- IMPLANT PICK-UP

integrated screw



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON TR-00021.8	2CON TR-00031.6
-----------------	-----------------

2CON TR-00021.8	2CON TR-00031.6
-----------------	-----------------

## 2-CONNECT®- SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 9.S3D1.800	2CON 9.S3D1.600
-----------------	-----------------

2CON 9.S3D1.800	2CON 9.S3D1.600
-----------------	-----------------

★  
★

## 2-CONNECT®- LAB ANALOG



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.La1.800	2CON 5.La1.600
----------------	----------------

2CON 5.La1.800	2CON 5.La1.600
----------------	----------------

★  
★

## 2-CONNECT®- DIM ANALOG



- Straight KS 61 =  $\varnothing$  1,8 mm
- Angled KS 62 =  $\varnothing$  1,6 mm

2CON 5.DIM.180	2CON 5.DIM.160
----------------	----------------

2CON 5.DIM.180	2CON 5.DIM.160
----------------	----------------

★  
★

## SLEEVE

for plaster model  
Stainless Steel



DIM 5.XSL.A30


DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# NT-Preform®

Milling blank for individual one-piece titanium abutments in CAM process



## BENEFITS:

- precise prefabricated implant interface
- optimal gingiva forming by two different gingiva heights
- individual abutment design by prosthetical terms (diameter, etc. )
- optimal interface protection by bilateral fixing in preform holder during milling process




## APPLICATION:

- primary telescopes on implants
- mesio-structures for crowns and bridges
- occlusal screwable structures



## TECHNICAL DETAILS:

- Titanium Grade 5 ELI



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA



# TABLE OF CONTENTS

NT CATALOGUE 2017-1

<b>1</b>	<b>TITANIUM BASE ABUTMENT</b>	<b>10 – 49</b>
<b>2</b>	<b>2-CONnect® ABUTMENT</b>	<b>50 – 117</b>
<b>3</b>	<b>NT-PREFORMS® ABUTMENT</b>	<b>118 – 147</b>
<b>4</b>	<b>DIM ANALOG</b>	<b>148 – 161</b>
<b>5</b>	<b>SURGICAL GUIDE SLEEVES</b>	<b>163 – 165</b>
<b>6</b>	<b>TOOLS &amp; DISCS</b>	<b>167 – 181</b>
<b>7</b>	<b>NT-iDent</b>	<b>182 – 189</b>
<b>8</b>	<b>SPECIFICATION</b>	<b>190 – 191</b>

## **BEG-SERIES – NEW**

is compatible to: BEGO Implant Systems® / Semados®  
S, RS-RX, RI-Line - - - - - **120**

## **BIO-SERIES – NEW**

is compatible to: BioHorizons® / internal- - - - - **121**

## **BRE-SERIES – NEW**

is compatible to: Bredent Medical® / Sky® - - - - - **122**

## **CAM-SERIES**

is compatible to: Altatec® / Camlog® - - - - - **123**

## **COL-SERIES**

is compatible to: Altatec® / Conelog® - - - - - **124**

## **E-SERIES**

is compatible to: Nobel Biocare™ / Replace Select®- - - - - **125**

## **F-SERIES**

is compatible to: Nobel Biocare™ / Nobel Active™ - - - - - **126**

## **I-SERIES**

is compatible to: Biomet 3i® / Osseotite® External Hex® - - - - - **126**

## **H-SERIES**

is compatible to: Biomet 3i® / Certain® - - - - - **127**

## **HIO-SERIES – NEW**

is compatible to: HIOSSEN® / OSSTEM TS® - - - - - **128**

## **K-SERIES**

is compatible to: Nobel Biocare™ / Brånemark® - - - - - **129**

## **L-SERIES**

is compatible to: Straumann / Bone Level®- - - - - **130**

## **MEX-SERIES – NEW**

is compatible to: Medentis Medical® / ICX®- - - - - **131**

## **MIC-SERIES – NEW**

is compatible to: MIS® / C1® - - - - - **132**

## **MIS-SERIES – NEW**

is compatible to: MIS® / SEVEN®- - - - - **133**

## **N-SERIES**

is compatible to: Straumann / SynOcta® - - - - - **134**

## **NEO-SERIES – NEW**

is compatible to: NEOSS Implant System® / NEOSS™ - - - - - **135**

## **R-SERIES**

is compatible to: Zimmer Dental / Tapered Screw-Vent® - - - - - **136**

## **S-SERIES**

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System OsseoSpeed® TX - - - - - **137**

## **SEV-SERIES – NEW**

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System™ EV - - - - - **138**

## **T-SERIES**

is compatible to: DENTSPLY Implants® / Xive® - - - - - **139**

## **THO-SERIES – NEW**

is compatible to: Thommen Medical® / SPI® - - - - - **140**

## **UPR-SERIES – NEW**

is compatible to: Sweden & Martina Implantology™ /  
Premium Kohno®- - - - - **141**

## **UTG-SERIES – NEW**

is compatible to: Sweden & Martina Implantology™ /  
Premium TG®- - - - - **142**

## **Holder fixture and Accessories**

- Holder fixture - - - - - **143**
- Accessories - - - - - **144**
- 3,5 mm Abutment grip- - - - - **145**
- 4,3 mm Abutment grip- - - - - **146**
- 5,0 mm Abutment grip- - - - - **147**

# BEG-SERIES

compatible to: BEGO Implant Systems® / Semados® S, RS-RX, RI-Line



**PLATFORM**

3,25 / 3,75 mm

4,1 mm

4,5 mm

5,5 mm

**NT-PREFORM®**

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm

BEG 10.Mi3.237.05

BEG 10.Mi4.100.05

BEG 10.Mi4.500.05

BEG 10.Mi5.500.05

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



BEG 5.La3.237

BEG 5.La4.100

BEG 5.La4.500

BEG 5.La5.500

★

**ABUTMENT GRIP**

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.300.000

W 12.300.000

★

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



BEG 9.S3D3.237

BEG 9.S3D4.100

BEG 9.S3D4.500

BEG 9.S3D5.500

★

**COLOURED MILLING SCREW**

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



BEG 6.Sc3.255

BEG 6.Sc3.255

BEG 6.Sc3.255

BEG 6.Sc3.255

★

**ABUTMENT SCREW**

Recommended tightening  
torques 30 Ncm  
Titanium Grade 5 ELI



BEG 603255

BEG 603255

BEG 603255

BEG 603255

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# BIO-SERIES

compatible to: BioHorizons® / internal



**PLATFORM**

3,0 mm

3,5 mm

4,5 mm

5,7 mm

**NT-PREFORM®**

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm

BIO 10.Mi3.000.05

BIO 10.Mi3.500.05

BIO 10.Mi4.500.05

BIO 10.Mi5.700.05

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



BIO 5.La3.000

BIO 5.La3.500

BIO 5.La4.500

BIO 5.La5.700

★

**ABUTMENT GRIP**

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.100.000

W 12.200.000

W 12.300.000

★

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



BIO 9.S3D3.000

BIO 9.S3D3.500

BIO 9.S3D4.500

BIO 9.S3D5.700

★

**COLOURED MILLING SCREW**

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



BIO 6.Sc3.057

BIO 6.Sc3.057

BIO 6.Sc3.057

BIO 6.Sc3.057

★

**ABUTMENT SCREW**

Recommended  
tightening torques  
30 Ncm  
Titanium Grade 5 ELI



BIO 603057

BIO 603057

BIO 603057

BIO 603057

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# BRE-SERIES

compatible to: Bredent Medical® / Sky®



**PLATFORM**

3,5 mm

4,0 mm

**NT-PREFORM®**

incl. coloured milling screw  
Titanium Grade 5 ELI




Gingiva Height 0,5 mm

BRE 10.Mi3.500.05

BRE 10.Mi4.000.05

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



BRE 5.La3.500

BRE 5.La4.000

★

**ABUTMENT GRIP**

for nt-Holder fixture  
Stainless Steel



W 12.200.000

W 12.200.000

★

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



BRE 9.S3D3.500

BRE 9.S3D4.000

★

**COLOURED MILLING SCREW**

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



BRE 6.Sc3.540

BRE 6.Sc3.540

★

**ABUTMENT SCREW**

Recommended  
tightening torques  
25 Ncm  
Titanium Grade 5 ELI



BRE 603540

BRE 603540

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# CAM-SERIES

compatible to: Altatec® / Camlog®



## PLATFORM

3,3 mm

3,8 mm

4,3 mm

5,0 mm

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm

CAM 10.Mi3.300.05

CAM 10.Mi3.800.05

CAM 10.Mi4.300.05

CAM 10.Mi5.000.05

★

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



CAM 5.La3.300

CAM 5.La3.800

CAM 5.La4.300

CAM 5.La5.060

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.100.000

W 12.200.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



CAM 9.S3D3.300

CAM 9.S3D3.800

CAM 9.S3D4.300

CAM 9.S3D5.060

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



CAM 6.Sc3.384

CAM 6.Sc3.384

CAM 6.Sc3.384

CAM 6.Sc5.060

★

## ABUTMENT SCREW

Recommended tightening  
torques 20 Ncm  
Titanium Grade 5 ELI



CAM 6033843

CAM 6033843

CAM 6033843

CAM 6150600

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# COL-SERIES

compatible to: Altatec® / Conelog®



3,3 mm



3,8 / 4,3 mm



5,0 mm

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height : 1,3 mm  
: 0,5 mm

COL 10.Mi3.300

COL 10.Mi3.843

COL 10.Mi5.000

COL 10.Mi3.300.05

COL 10.Mi3.843.05

COL 10.Mi5.000.05

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



COL 5.La3.300

COL 5.La3.843

COL 5.La5.000

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



COL 9.S3D3.300

COL 9.S3D3.843

COL 9.S3D5.000

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



COL 6.Sc3.343

COL 6.Sc3.343

COL 6.Sc5.000

★

## ABUTMENT SCREW

Recommended  
tightening torques 20 Ncm  
Titanium Grade 5 ELI



COL 603343

COL 603343

COL 605000

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# E-SERIES

compatible to: Nobel Biocare™ / Replace Select®



## PLATFORM

3,5 mm NP

4,3 mm RP

5,0 mm WP

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height

1,3 mm

0,5 mm

E 10.Mi3.500

E 10.Mi4.300

E 10.Mi5.000

★

E 10.Mi3.500.05

E 10.Mi4.300.05

E 10.Mi5.000.05

★

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



E 5.La3.500

E 5.La4.300

E 5.La5.000

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



E 9.S3D3.500

E 9.S3D4.300

E 9.S3D5.000

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



E 6.Sc3.500

E 6.Sc4.350

E 6.Sc4.350

★

## ABUTMENT SCREW

Recommended tightening  
torques 35 Ncm  
Titanium Grade 5 ELI



E 60

E 61

E 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# F-SERIES

compatible to: Nobel Biocare™ / Nobel Active™

# I-SERIES

compatible to Biomet 3i® / Osseotite® External Hex®



## PLATFORM

3,5 mm NP

4,3 / 5,0 mm RP

4,1 mm

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height

1,3 mm

0,5 mm

F 10.Mi3.500

F 10.Mi4.350

I 10.Mi4.100

F 10.Mi3.500.05

F 10.Mi4.350.05

I 10.Mi4.100.05

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



F 5.La3.500

F 5.La4.350

I 5.La4.100

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.200.000

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



F 9.S3D3.500

F 9.S3D4.350

I 9.S3D4.150

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



F 6.Sc3.500

F 6.Sc4.350

I 6.Sc4.100

## ABUTMENT SCREW

Recommended tightening  
torques F-Series: NP = 25 Ncm  
F-Series: RP = 35 Ncm  
I-Series: 35 Ncm  
Titanium Grade 5 ELI



F 60

F 61

I 61

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# H-SERIES

compatible to: Biomet 3i® / Certain®



## PLATFORM

3,4 mm NP

4,1 mm RP

5,0 mm WP

## NT-PREFORM®

incl. coloured Milling Screw  
Titanium Grade 5 ELI



Gingiva Height

1,3 mm

0,5 mm

H 10.Mi3.400

H 10.Mi4.100

H 10.Mi5.000

★

H 10.Mi3.400.05

H 10.Mi4.100.05

H 10.Mi5.000.05

★

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



H 5.La3.400

H 5.La4.100

H 5.La5.000

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



H 9.S3D3.400

H 9.S3D4.150

H 9.S3D4.150

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



H 6.Sc3.450

H 6.Sc3.450

H 6.Sc3.450

★

## ABUTMENT SCREW

Recommended  
tightening torques  
20 Ncm  
Titanium Grade 5 ELI



H 60

H 60

H 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# HIO-SERIES

compatible to: HIOSSEN® / OSSTEM TS®



**PLATFORM**

3,5 mm

4,0 - 6,0 mm

**NT-PREFORM®**

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm

HIO 10.Mi3.500.05

HIO 10.Mi4.060.05

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



HIO 5.La3.500

HIO 5.La4.060

★

**ABUTMENT GRIP**

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

★

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



HIO 9.S3D3.500

HIO 9.S3D4.060

★

**COLOURED MILLING SCREW**

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



HIO 6.Sc3.500

HIO 6.Sc4.060

★

**ABUTMENT SCREW**

Recommended tightening  
torques 3,5 mm = 20 Ncm  
4,0 - 6,0 mm = 30 Ncm  
Titanium Grade 5 ELI



HIO 603500

HIO 604060

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# K-SERIES

compatible to: Nobel Biocare™ / Brånemark®



## PLATFORM

3,5 mm

4,1 mm

5,1 mm

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height

1,3 mm

0,5 mm

K 10.Mi3.500

K 10.Mi4.100

K 10.Mi5.100

★

K 10.Mi3.500.05

K 10.Mi4.100.05

K 10.Mi5.100.05

★

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



K 5.La3.500

K 5.La4.100

K 5.La5.100

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



K 9.S3D3.500

K 9.S3D4.100

K 9.S3D5.100

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



K 6.Sc3.500

K 6.Sc4.100

K 6.Sc5.100

★

## ABUTMENT SCREW

Recommended  
tightening torques 35 Ncm  
Titanium Grade 5 ELI



K 60

K 61

K 62

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# L-SERIES

compatible to: Straumann / Bone Level®



## PLATFORM

3,3 mm NC

4,1 / 4,8 mm RC

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height : 1,3 mm  
: 0,5 mm

L 10.Mi3.300

L 10.Mi4.148

L 10.Mi3.300.05

L 10.Mi4.148.05

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



L 5.La3.300

L 5.La4.148

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



L 9.S3D3.300

L 9.S3D4.148

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



L 6.Sc3.341

L 6.Sc3.341

★

## ABUTMENT SCREW

Recommended  
tightening torques  
35 Ncm  
Titanium Grade 5 ELI



L 60

L 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# MEX-SERIES

compatible to: Medentis Medical® / ICX®



## PLATFORM

3,45 - 4,8 mm

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI




Gingiva Height 0,5 mm

MEX 10.Mi3.748.05

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



MEX 5.La3.748



## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.200.000



## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



MEX 9.S3D3.748



## MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



MEX 6.Sc4.148



## ABUTMENT SCREW

Recommended  
tightening torques 30 Ncm  
Titanium Grade 5 ELI



MEX 603748

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# MIC-SERIES

compatible to: MIS® / C1®



3,3 mm NP



3,75 / 4,2 mm SP



5,0 mm WP

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm


MIC 10.Mi3.300.05

MIC 10.Mi3.742.05

MIC 10.Mi5.000.05

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



MIC 5.La3.300

MIC 5.La3.742

MIC 5.La5.000

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



MIC 9.S3D3.300

MIC 9.S3D3.742

MIC 9.S3D5.000

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



MIC 6.Sc3.750

MIC 6.Sc3.750

MIC 6.Sc3.750

★

## ABUTMENT SCREW

Recommended  
tightening torques 30 Ncm  
Titanium Grade 5 ELI



MIC 603300

MIC 603750

MIC 603750

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# MIS-SERIES

compatible to: MIS® / SEVEN®



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**NT-PREFORM®**

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm

MIS 10.Mi3.300.05

MIS 10.Mi3.742.05

MIS 10.Mi5.000.05

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



MIS 5.La3.300

MIS 5.La3.742

MIS 5.La5.000

★

**ABUTMENT GRIP**

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.300.000

★

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



MIS 9.S3D3.300

MIS 9.S3D3.742

MIS 9.S3D5.000

★

**COLOURED MILLING SCREW**

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



MIS 6.Sc3.300

MIS 6.Sc3.750

MIS 6.Sc3.750

★

**ABUTMENT SCREW**

Recommended  
tightening torques 30 Ncm  
Titanium Grade 5 ELI



MIS 603300

MIS 603750

MIS 603750

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# N-SERIES

compatible to: Straumann / SynOcta®



## PLATFORM

3,5 mm NN

4,8 mm RN

4,8 mm RN

6,5 mm WN

6,5 mm WN

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



without shoulder

with shoulder

without shoulder

with shoulder

Gingiva Height

1,3 mm

0,5 mm

N 10.Mi3.500

N 10.Mi4.800

N 10.Mi4.805

N 10.Mi6.500

N 10.Mi6.505

★

N 10.Mi3.500.05

—

N 10.Mi4.805.05

—

N 10.Mi6.505.05

★

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



N 5.La3.500

N 5.La4.800

N 5.La4.800

N 5.La6.500

N 5.La6.500

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.200.000

W 12.300.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



N 9.S3D3.500

N 9.S3D4.800

N 9.S3D4.800

N 9.S3D6.500

N 9.S3D6.500

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



N 6.Sc3.500

N 6.Sc4.865

N 6.Sc4.865

N 6.Sc4.865

N 6.Sc4.865

★

## ABUTMENT SCREW

Recommended  
tightening torques 35 Ncm  
Titanium Grade 5 ELI



N 60

N 62

N 62

N 62

N 62


★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# NEO-SERIES

compatible to: *NEOSS Implant System® / NEOSS™*



## PLATFORM

3,5 - 5,5 mm

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm

NEO 10.Mi3.555.05

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



NEO 5.La3.555

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.200.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



NEO 9.S3D3.555

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



NEO 6.Sc3.555

★

## ABUTMENT SCREW

Recommended  
tightening torques 30 Ncm  
Titanium Grade 5 ELI



NEO 603555

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# R-SERIES

compatible to: Zimmer Dental / Tapered Screw-Vent®



## PLATFORM

3,5 mm

4,5 mm

5,7 mm

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height

1,3 mm

0,5 mm

R 10.Mi3.500

R 10.Mi4.500

R 10.Mi5.700

★

R 10.Mi3.500.05

R 10.Mi4.500.05

R 10.Mi5.700.05

★

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



R 5.La3.500

R 5.La4.500

R 5.La5.700

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



R 9.S3D3.500

R 9.S3D4.500

R 9.S3D5.700

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



R 6.Sc3.557

R 6.Sc3.557

R 6.Sc3.557

★

## ABUTMENT SCREW

Recommended  
tightening torques 30 Ncm  
Titanium Grade 5 ELI



R 60

R 60

R 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# S-SERIES

compatible to: DENTSPLY Implants® / Astra Tech Implant System Osseospeed® TX



## PLATFORM

3,5 / 4,0 mm

4,5 / 5,0 mm

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height

1,3 mm

0,5 mm

S 10.Mi3.540

S 10.Mi4.550

★

S 10.Mi3.540.05

S 10.Mi4.550.05

★

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



groove

groove

S 5.La3.540

S 5.La4.550

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



S 9.S3D3.540

S 9.S3D4.550

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



S 6.Sc3.540

S 6.Sc4.550

★

## ABUTMENT SCREW

Recommended  
tightening torques 25 Ncm  
Titanium Grade 5 ELI



S 60




































S 61

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# SEV-SERIE

compatible to: DENTSPLY Implants® / Astra Tech Implant System™ EV

					
<b>PLATFORM</b>	3,0 mm	3,6 mm	4,2 mm	4,8 mm	5,4 mm
<b>NT-PREFORM®</b> incl. coloured milling screw Titanium Grade 5 ELI					
Gingiva Height 0,5 mm	SEV 10.Mi3.000.05	SEV 10.Mi3.600.05	SEV 10.Mi4.200.05	SEV 10.Mi4.800.05	SEV 10.Mi5.400.05
<b>NT-MILL LAB ANALOG</b> for nt-Preform® Stainless Steel					
	SEV 5.La3.000	SEV 5.La3.600	SEV 5.La4.200	SEV 5.La4.800	SEV 5.La5.400 ★
<b>ABUTMENT GRIP</b> for nt-Holder fixture Stainless Steel					
	W 12.100.000	W 12.100.000	W 12.200.000	W 12.300.000	W 12.300.000 ★
<b>SCAN BODY 3D-GUIDE®</b> for intra + extra oral scanning					
	SEV 9.S3D3.000	SEV 9.S3D3.600	SEV 9.S3D4.200	SEV 9.S3D4.800	SEV 9.S3D5.400 ★
<b>COLOURED MILLING SCREW</b> for nt-Preform® Recommended tightening torques 10 Ncm					
	SEV 6.Sc3.000	SEV 6.Sc3.600	SEV 6.Sc4.200	SEV 6.Sc4.854	SEV 6.Sc4.854 ★
<b>ABUTMENT SCREW</b> Recommended tightening torques 25 Ncm Titanium Grade 5 ELI					
	SEV 603000	SEV 603600	SEV 604200	SEV 604854	SEV 604854

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# T-SERIES

compatible to: DENTSPLY Implants® / Xive®



3,4 mm



3,8 mm



4,5 mm



5,5 mm

## PLATFORM

## NT-PREFORM®

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height : 1,3 mm  
: 0,5 mm

T 10.Mi3.400

T 10.Mi3.800

T 10.Mi4.500

T 10.Mi5.500

★

T 10.Mi3.400.05

T 10.Mi3.800.05

T 10.Mi4.500.05

T 10.Mi5.500.05

★

## NT-MILL LAB ANALOG

for nt-Preform®  
Stainless Steel



T 5.La3.400

T 5.La3.800

T 5.La4.500

T 5.La5.500

★

## ABUTMENT GRIP

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.200.000

W 12.300.000

★

## SCAN BODY 3D-GUIDE®

for intra + extra  
oral scanning



T 9.S3D3.400

T 9.S3D3.800

T 9.S3D4.555

T 9.S3D4.555

★

## COLOURED MILLING SCREW

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



T 6.Sc3.455

T 6.Sc3.455

T 6.Sc3.455

T 6.Sc3.455

★

## ABUTMENT SCREW

Recommended  
tightening torques 25 Ncm  
Titanium Grade 5 ELI



T 60

T 60

T 60

T 60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# THO-SERIES

compatible to: Thommen Medical® / SPI®



**PLATFORM**

3,5 mm      4,0 mm      4,5 mm      5,0 mm      6,0 mm

**NT-PREFORM®**

ncl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm    THO 10.Mi3.500.05    THO 10.Mi4.000.05    THO 10.Mi4.500.05    THO 10.Mi5.000.05    THO 10.Mi6.000.05

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



THO 5.La3.500    THO 5.La4.000    THO 5.La4.500    THO 5.La5.000    THO 5.La6.000 ★

**ABUTMENT GRIP**

for nt-Holder fixture  
Stainless Steel



W 12.100.000    W 12.200.000    W 12.200.000    W 12.300.000    W 12.300.000 ★

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



THO 9.S3D3.500    THO 9.S3D4.000    THO 9.S3D4.500    THO 9.S3D5.000    THO 9.S3D6.000 ★

**COLOURED MILLING SCREW**

for nt-Preform®  
Recommended tightening  
torques 10 Ncm  
Recommended screwdriver  
W 11.TH0.MIL 4-socket



THO 6.Sc3.500    THO 6.Sc4.060    THO 6.Sc4.060    THO 6.Sc4.060    THO 6.Sc4.060 ★

**ABUTMENT SCREW**

Recommended tightening  
torques 3,5 mm = 15 Ncm  
4,0 - 6,0 mm = 25 Ncm  
Titanium Grade 5 ELI



THO 603500    THO 604060    THO 604060    THO 604060    THO 604060

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# UPR-SERIES

compatible to: Sweden & Martina Implantology™ / Premium Kohno®



**PLATFORM**

3,3 mm

3,8 mm

4,25 mm

5,0 mm

**NT-PREFORM®**

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm

UPR 10.Mi3.300.05

UPR 10.Mi3.800.05

UPR 10.Mi4.200.05

UPR 10.Mi5.000.05

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



UPR 5.La3.300

UPR 5.La3.800

UPR 5.La4.200

UPR 5.La5.000

★

**ABUTMENT GRIP**

for nt-Holder fixture  
Stainless Steel



W 12.100.000

W 12.200.000

W 12.200.000

W 12.300.000

★

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



UPR 9.S3D3.300

UPR 9.S3D3.800

UPR 9.S3D4.200

UPR 9.S3D5.000

★

**COLOURED MILLING SCREW**

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



UPR 6.Sc3.338

UPR 6.Sc3.338

UPR 6.Sc4.250

UPR 6.Sc4.250

★

**ABUTMENT SCREW**

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



UPR 603338

UPR 603338

UPR 604250

UPR 604250

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# UTG-SERIES

compatible to: Sweden & Martina Implantology™ / Premium TG®



**PLATFORM**

3,3 - 4,25 mm

5,0 mm

**NT-PREFORM®**

incl. coloured milling screw  
Titanium Grade 5 ELI



Gingiva Height 0,5 mm

UTG 10.Mi3.342.05

UTG 10.Mi5.000.05

**NT-MILL LAB ANALOG**

for nt-Preform®  
Stainless Steel



UTG 5.La3.342

UTG 5.La5.000

★

**ABUTMENT GRIP**

for nt-Holder fixture  
Stainless Steel



W 12.200.000

W 12.300.000

★

**SCAN BODY 3D-GUIDE®**

for intra + extra  
oral scanning



UTG 9.S3D3.342

UTG 9.S3D5.000

★

**COLOURED MILLING SCREW**

for nt-Preform®  
Recommended tightening  
torques 10 Ncm



UTG 6.Sc3.342

UTG 6.Sc5.000

★

**ABUTMENT SCREW**

Recommended tightening  
torques 25 Ncm  
Titanium Grade 5 ELI



UTG 603342

UTG 605000


Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# SETS

for several machines

- Avamill-Chrome®
- Datron D5®
- Datron M7®
- Datron NT98®
- Dental concept systems® DC5
- DooWoon
- Dyamach® DT 2
- GF Agie Charmilles
- Mikron HSM 200 +
- HSM 400
- HINT-ELS
- IMES-ICORE®
- MB Maschinen
- Organical
- Röders RXD®
- Sauer ULTRASONIC 20®
- Willemin-Macodel®
- Wissner
- ZFX
- VHF Camfature



## CONTENT

NO.	ART. NO.	DESCRIPTION	QUANTITY	
1	customer request	nt-Holder fixture	1 pc.	★
2	customer request	Abutment grip diameter 3,5 mm, 4,3 mm or 5,0 mm	2 pcs.	★
3	W 12.Sc1.000	Holding screw No. 1 (Abutment grip screw), Set (content 4 pcs.)	1 pc.	★
4	W 12.Sc2.000	Holding screw No. 2 (holding fixture grip), Set (content 4 pcs.)	1 pc.	★
5	W 12.We1.000	Tool No. 1 (Abutment grip screw)	1 pc.	★
6	W 12.We2.000	Tool No. 2 (Holder fixture)	1 pc.	★
7	customer request	nt-Mill Lab Analog	6 pcs.	★
8	customer request	nt-Preform®, incl. coloured milling screw	6 pcs.	★
9	customer request	Abutment Screw	6 pcs.	★










Notice: Products indicated with ® and ™ are registered brand names of the respective manufacturers.  
 Products indicated with ★ are available in the USA

# ACCESSORIES

NT-Preform® Accessories & Holder fixture-sets



## CONTENT NT-PREFORM® ACCESSORIES

	ART. NO.	DESCRIPTION	
	W 12.100.000	Abutment grip diameter 3,5 mm, 1pc.	★
	W 12.200.000	Abutment grip diameter 4,3 mm, 1pc.	★
	W 12.300.000	Abutment grip diameter 5,0 mm, 1pc.	★
	W 12.Ka0.000	Calibration pin for nt-Preform holder fixture imes-icore®	★
	W 12.Ka0.140	Calibration pin for nt-Preform holder fixture imes-icore® 140	★
	W 12.CS0.000	Replacement of cover strip for abutment grip incl. 2 screws	★
	W 12.Sc0.000	Replacement screws for holder fixture contains: W 12.Sc1.000, W 12.Sc2.000 and grub screws for Abutment grip	★
	W 12.WS0.000	Tools for holder fixture contains: W 12.We1.000, W 12.We2.000, W 12.We3.000	★
	W 11.THO.MIL	SCREWDRIVER incl. ISO-Shaft for Torque Ratchet for coloured milling screw THO-Series, 4-socket	★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# ABUTMENT GRIP

3,5 mm  W 12.100.000



## ABUTMENT GRIP 3,5 mm nt-Mill Lab Analogs

NO.	ART. NO.	SYSTEM	DESCRIPTION	
1	BEG 5.La3.237	BEGO Implant Systems® / Semados® S, RS-RX, RI-Line	nt-Mill Lab Analog 3,2 / 3,7 mm	
2	BIO 5.La3.000	BioHorizons® / internal	nt-Mill Lab Analog 3,0 m	
3	BIO 5.La3.500	BioHorizons® / internal	nt-Mill Lab Analog 3,5 mm	
4	CAM 5.La3.300	Altatec® / Camlog®	nt-Mill Lab Analog 3,3 mm	★
5	CAM 5.La3.800	Altatec® / Camlog®	nt-Mill Lab Analog 3,8 mm	★
6	COL 5.La3.300	Altatec® / Conelog®	nt-Mill Lab Analog 3,3 mm	
7	E 5.La3.500	Nobel Biocare / Replace Select®	nt-Mill Lab Analog 3,5 mm NP	★
8	F 5.La3.500	Nobel Biocare / Nobel Active™	nt-Mill Lab Analog 3,5 mm NP	★
9	H 5.La3.400	Biomet 3i® / Certain®	nt-Mill Lab Analog 3,4 mm	★
10	HIO 5.La3.500	HIOSEN® / OSSTEM TS®	nt-Mill Analog 3,5mm	
11	K 5.La3.500	Nobel Biocare™ / Brånemark®	nt-Mill Lab Analog 3,5 mm	★
12	L 5.La3.300	Straumann / Bone Level®	nt-Mill Lab Analog 3,3 mm NC	★
13	MIC 5.La3.300	MIC® / C1®	nt-Mill Analog 3,3 mm	
14	MIS 5.La3.300	MIS® / SEVEN®	nt-Mill Analog 3,3 mm	
15	N 5.La3.500	Straumann / SynOcta®	nt-Mill Lab Analog 3,5 mm NN	★
16	R 5.La3.500	Zimmer Dental / Tapered Screw-Vent®	nt-Mill Lab Analog 3,5 mm	★
17	S 5.La3.540	DENTSPLY Implants® / Astra Tech Implant System OsseoSpeed® TX	nt-Mill Lab Analog 3,5 / 4,0 mm	★
18	SEV 5.La3.000	DENTSPLY Implants® / Astra Tech Implant System™ EV	nt-Mill Lab Analog 3,0 mm	
19	SEV 5.La3.600	DENTSPLY Implants® / Astra Tech Implant System™ EV	nt-Mill Lab Analog 3,6 mm	
20	T 5.La3.400	Dentsply-Friadent Frialit/Xive®	nt-Mill Lab Analog 3,4 mm	★
21	THO 5.La3.500	Thommen Medical® / SPI®	nt-Mill Analog 3,5mm	
22	UPR 5.La3.300	Sweden & Martina Implantology™ / Premium Kohno®	nt-Mill Analog 3,3 mm	

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# ABUTMENT GRIP

4,3 mm  W 12.200.000



## ABUTMENT GRIP 4,3 mm nt-Mill Lab Analogs

NO.	ART. NO.	SYSTEM	DESCRIPTION	
1	BEG 5.La4.100	BEGO Implant Systems® / Semados® S, RS-RX, RI-Line	nt-Mill Lab Analog 4,1 mm	
2	BIO 5.La4.500	BioHorizons® / internal	nt-Mill Lab Analog 4,5 mm	
3	BRE 5.La3.540	Bredent Medical® / Sky®	nt-Mill Lab Analog 3,5 / 4,0 mm	
4	CAM 5.La4.300	Altatec® / Camlog®	nt-Mill Lab Analog 4,3 mm	★
5	COL 5.La3.843	Altatec® / Conelog®	nt-Mill Lab Analog 3,8 / 4,3 mm	
6	E 5.La4.300	Nobel Biocare / Replace Select®	nt-Mill Lab Analog 4,3 mm RP	★
7	F 5.La4.350	Nobel Biocare / Nobel Active™	nt-Mill Lab Analog 4,3/5,0 mm RP	★
8	H 5.La4.100	Biomet 3i® / Certain®	nt-Mill Lab Analog 4,1 mm	★
9	HIO 5.La4.060	HIOSEN® / OSSTEM TS®	nt-Mill Analog 4,0-6,0mm	
10	I 5.La4.100	Biomet 3i® / Osseotite® External Hex®	nt-Mill Lab Analog 4,1 mm	★
11	K 5.La4.100	Nobel Biocare™ / Brånemark®	nt-Mill Lab Analog 4,1 mm	★
12	L 5.La4.148	Straumann / Bone Level®	nt-Mill Lab Analog 4,1 / 4,8 mm RC	★
13	MEX 5.La4.148	Medentis Medical® / ICX®	nt-Mill Analog 4,1/4,8 mm	
14	MIC 5.La3.742	MIC® / C1®	nt-Mill Analog 3,75/4,2 mm	
15	MIS 5.La3.742	MIS® / SEVEN®	nt-Mill Analog 3,75/4,2 mm	
16	N 5.La4.800	Straumann / SynOcta®	nt-Mill Lab Analog 4,8 mm RN	★
17	NEO 5.La3.555	NEOSS Implant System® / NEOSS™	nt-Mill Analog 3,5-5,5 mm	
18	R 5.La4.500	Zimmer Dental / Tapered Screw-Vent®	nt-Mill Lab Analog 4,5 mm	★
19	S 5.La4.550	DENTSPLY Implants® / Astra Tech Implant System OsseoSpeed® TX	nt-Mill Lab Analog 4,5 / 5,0 mm	★
20	SEV 5.La4.200	DENTSPLY Implants® / Astra Tech Implant System™ EV	nt-Mill Lab Analog 4,2 mm	
21	T 5.La3.800	DENTSPLY Implants® / Xive®	nt-Mill Lab Analog 3,8 mm	★
22	T 5.La4.500	DENTSPLY Implants® / Xive®	nt-Mill Lab Analog 4,5 mm	★
23	THO 5.La4.000	Thommen Medical® / SPI®	nt-Mill Analog 4,0 mm	
24	THO 5.La4.500	Thommen Medical® / SPI®	nt-Mill Analog 4,5 mm	
25	UPR 5.La3.800	Sweden & Martina Implantology™ / Premium Kohno®	nt-Mill Analog 3,8 mm	
26	UPR 5.La4.200	Sweden & Martina Implantology™ / Premium Kohno®	nt-Mill Analog 4,25 mm	
27	UTG 5.La3.342	Sweden & Martina Implantology™ / Premium TG®	nt-Mill Analog 3,3-4,25 mm	

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA

# ABUTMENT GRIP

5,0 mm  W 12.300.000




## ABUTMENT GRIP 5,0 mm nt-Mill Lab Analogs

NO.	ART. NO.	SYSTEM	DESCRIPTION	
1	BEG 5.La4.500	BEGO Implant Systems® / Semados® S, RS-RX, RI-Line	nt-Mill Lab Analog 4,5 mm	
2	BEG 5.La5.500	BEGO Implant Systems® / Semados® S, RS-RX, RI-Line	nt-Mill Lab Analog 5,5 mm	
3	BIO 5.La5.700	BioHorizons® / internal	nt-Mill Lab Analog 5,7 mm	
4	CAM 5.La5.060	Altatec® / Camlog®	nt-Mill Lab Analog 5,0 mm	★
5	COL 5.La5.000	Altatec® / Conelog®	nt-Mill Lab Analog 5,0 mm	
6	E 5.La5.000	Nobel Biocare / Replace Select®	nt-Mill Lab Analog 5,0 mm WP	★
7	H 5.La5.000	Biomet 3i® / Certain®	nt-Mill Lab Analog 5,0 mm	★
8	K 5.La5.100	Nobel Biocare™ / Brånemark®	nt-Mill Lab Analog 5,1 mm	★
9	MIC 5.La5.000	MIC® / C1®	nt-Mill Analog 5,0 mm	
10	MIS 5.La5.000	MIS® / SEVEN®	nt-Mill Analog 5,0 mm	
11	N 5.La6.500	Straumann / SynOcta®	nt-Mill Lab Analog 6,5 mm WN	★
12	R 5.La5.700	Zimmer Dental / Tapered Screw-Vent®	nt-Mill Lab Analog 5,7 mm	★
13	SEV 5.La4.800	DENTSPLY Implants® / Astra Tech Implant System™ EV	nt-Mill Lab Analog 4,8 mm	
14	SEV 5.La5.400	DENTSPLY Implants® / Astra Tech Implant System™ EV	nt-Mill Lab Analog 5,4 mm	
15	T 5.La5.500	DENTSPLY Implants® / Xive®	nt-Mill Lab Analog 5,5 mm	★
16	THO 5.La5.000	Thommen Medical® / SPI®	nt-Mill Analog 5,0 mm	
17	THO 5.La6.000	Thommen Medical® / SPI®	nt-Mill Analog 6,0 mm	
18	UPR 5.La5.000	Sweden & Martina Implantology™ / Premium Kohno®	nt-Mill Analog 5,00 mm	
19	UTG 5.La5.000	Sweden & Martina Implantology™ / Premium TG®	nt-Mill Analog 5,0 mm	

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# DIM\* ANALOG

\*Digital Implant Model ANALOG | Available for 24 implant systems in the nt-IQ library



## FEATURES:

- implant analog for digital model manufacturing in the model builder library
- two-piece repositionable implant analog
- precise positioning
- positional adjustment possible
- analog design supports precise repositioning of removable gingiva mask



## APPLICATION:

- for model manufacturing in digital workflow



## TECHNICAL DETAILS:

- Stainless Steel
- Titanium Grade 5 ELI



**INTERNATIONAL  
PATENT PENDING**



**DIM PARALLEL DRILL  
FOR PLASTER MODEL**



W 16.DIM.000

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with \* are available in the USA 

# TABLE OF CONTENTS

NT CATALOGUE 2017-1

<b>1</b>	<b>TITANIUM BASE ABUTMENT</b>	10 – 49
<b>2</b>	<b>2-CONnect® ABUTMENT</b>	50 – 117
<b>3</b>	<b>NT-PREFORMS® ABUTMENT</b>	118 – 147
<b>4</b>	<b>DIM ANALOG</b>	148 – 161
<b>5</b>	<b>SURGICAL GUIDE SLEEVES</b>	163 – 165
<b>6</b>	<b>TOOLS &amp; DISCS</b>	167 – 181
<b>7</b>	<b>NT-iDent</b>	182 – 189
<b>8</b>	<b>SPECIFICATION</b>	190 – 191

## **BEG-SERIES – NEW**

is compatible to: BEGO Implant Systems® / Semados®  
S, RS-RX, RI-Line - - - - - 150

## **BIO-SERIES – NEW**

is compatible to: BioHorizons® / internal- - - - - 150

## **BRE-SERIES – NEW**

is compatible to: Bredent Medical® / Sky® - - - - - 151

## **CAM-SERIES**

is compatible to: Altatec® / Camlog® - - - - - 151

## **COL-SERIES**

is compatible to: Altatec® / Conelog® - - - - - 152

## **E-SERIES**

is compatible to: Nobel Biocare™ / Replace Select®- - - - - 152

## **F-SERIES**

is compatible to: Nobel Biocare™ / Nobel Active™ - - - - - 153

## **H-SERIES**

is compatible to: Biomet 3i® / Certain® - - - - - 153

## **HIO-SERIES – NEW**

is compatible to: HIOSSEN® / OSSTEM TS® - - - - - 154

## **I-SERIES**

is compatible to: Biomet 3i® / Osseotite® External Hex® - - 154

## **K-SERIES**

is compatible to: Nobel Biocare™ / Brånemark® - - - - - 155

## **L-SERIES**

is compatible to: Straumann / Bone Level®- - - - - 155

## **MEX-SERIES – NEW**

is compatible to: Medentis Medical® / ICX®- - - - - 156

## **MIC-SERIES – NEW**

is compatible to: MIS® / C1® - - - - - 156

## **MIS-SERIES – NEW**

is compatible to: MIS® / SEVEN®- - - - - 157

## **N-SERIES**

is compatible to: Straumann / SynOcta® - - - - - 157

## **NEO-SERIES – NEW**

is compatible to: NEOSS Implant System® / NEOSS™ - - - - - 158

## **R-SERIES**

is compatible to: Zimmer Dental / Tapered Screw-Vent® - - 158

## **S-SERIES**

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System OsseoSpeed® TX - - - - - 159

## **SEV-SERIES – NEW**

is compatible to: DENTSPLY Implants® /  
Astra Tech Implant System™ EV - - - - - 159

## **T-SERIES**

is compatible to: DENTSPLY Implants® / Xive®- - - - - 160

## **THO-SERIES – NEW**

is compatible to: Thommen Medical® / SPI® - - - - - 160

## **UPR-SERIES – NEW**

is compatible to: Sweden & Martina Implantology™ /  
Premium Kohno®- - - - - 161

## **UTG-SERIES – NEW**


is compatible to: Sweden & Martina Implantology™ /  
Premium TG®- - - - - 161



**NEW**

# BEG-SERIES DIM ANALOG





compatible to: BEGO Implant Systems® / Semados® S, RS-RX, RI-Line

					
<b>PLATFORM</b>	3,25 / 3,75 mm	4,1 mm	4,5 mm	5,5 mm	
					
<b>DIM ANALOG</b>	BEG 5.DIM.323	BEG 5.DIM.410	BEG 5.DIM.450	BEG 5.DIM.550	★
					
<b>SLEEVE</b> for plaster model Stainless Steel	DIM 5.XSL.A20	DIM 5.XSL.A20	DIM 5.XSL.A30	DIM 5.XSL.A30	★

# BIO-SERIES DIM ANALOG

compatible to: BioHorizons® / internal

**NEW**

					
<b>PLATFORM</b>	3,0 mm	3,5 mm	4,5 mm	5,7 mm	
					
<b>DIM ANALOG</b>	BIO 5.DIM.300	BIO 5.DIM.350	BIO 5.DIM.450	BIO 5.DIM.570	★
					
<b>SLEEVE</b> for plaster model Stainless Steel	DIM 5.XSL.A10	DIM 5.XSL.A10	DIM 5.XSL.A30	DIM 5.XSL.A60	★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 



# BRE-SERIES DIM ANALOG

compatible to: *Bredent Medical® / Sky®*



**PLATFORM**

3,5 mm

4,0 mm

**DIM ANALOG**



BRE 5.DIM.350

BRE 5.DIM.400



**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A20

DIM 5.XSL.A20



# CAM-SERIES DIM ANALOG

compatible to: *Altatec® / Camlog®*



**PLATFORM**

3,3 mm

3,8 mm

4,3 mm

5,0/6,0 mm

**DIM ANALOG**



CAM 5.DIM.330

CAM 5.DIM.380

CAM 5.DIM.430

CAM 5.DIM.506



**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A40

DIM 5.XSL.A40

DIM 5.XSL.A50



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# COL-SERIES DIM ANALOG

compatible to: Altatec® / Conelog®



## PLATFORM

3,3 mm

3,8 / 4,3 mm

5,0 mm

## DIM ANALOG



COL 5.DIM.330

COL 5.DIM.384

COL 5.DIM.500

★

## SLEEVE

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A30

★

# E-SERIES DIM ANALOG

compatible to: Nobel Biocare™ / Replace Select®



## PLATFORM

3,5 mm NP

4,3 mm RP

5,0 mm WP

6,0 mm

## DIM ANALOG



E 5.DIM.350

E 5.DIM.430

E 5.DIM.500

E 5.DIM.600

★

## SLEEVE

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A30

DIM 5.XSL.A60

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# F-SERIES DIM ANALOG

compatible to: Nobel Biocare™ / Nobel Active™



**PLATFORM**

3,5 mm NP

4,3 / 5,0 mm RP

**DIM ANALOG**



F 5.DIM.350

F 5.DIM.435

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

★

# H-SERIES DIM ANALOG

compatible to: Biomet 3i® / Certain®



**PLATFORM**

3,4 mm NP

4,1 mm RP

5,0 mm WP

**DIM ANALOG**



H 5.DIM.340

H 5.DIM.410

H 5.DIM.500

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

**NEW**

# HIO-SERIES DIM ANALOG

compatible to: HIOSSEN® / OSSTEM TS®



**PLATFORM**

3,5 mm

4,0 - 6,0 mm

**DIM ANALOG**



HIO 5.DIM.350

HIO 5.DIM.406

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

★

# I-SERIES DIM ANALOG

compatible to: Biomet 3i® / Osseotite® External Hex®



**PLATFORM**

3,4 mm

4,1 mm

5,0 mm

**DIM ANALOG**



I 5.DIM.340

I 5.DIM.410

I 5.DIM.500

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# K-SERIES DIM ANALOG

compatible to: Nobel Biocare™ / Brånemark®



**PLATFORM**

3,5 mm

4,1 mm

5,1 mm

**DIM ANALOG**



K 5.DIM.350

K 5.DIM.410

K 5.DIM.510

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A30

★

# L-SERIES DIM ANALOG

compatible to: Straumann / Bone Level®



**PLATFORM**

3,3 mm NC

4,1 / 4,8 mm RC

**DIM ANALOG**



L 5.DIM.330

L 5.DIM.414

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

NEW

# MEX-SERIES DIM ANALOG

compatible to: Medentis Medical® / ICX®



**PLATFORM**

3,45 - 4,8 mm

**DIM ANALOG**



MEX 5.DIM.414

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A20

★

# MIC-SERIES DIM ANALOG

compatible to: MIS® / C1®

NEW



**PLATFORM**

3,3 mm NP

3,75 / 4,2 mm SP

5,0 mm WP

**DIM ANALOG**



MIC 5.DIM.330

MIC 5.DIM.374

MIC 5.DIM.500

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA










# MIS-SERIES DIM ANALOG

compatible to: MIS® / SEVEN®

				
<b>PLATFORM</b>	3,3 mm NP	3,75 / 4,2 mm SP	5,0 mm WP	
<b>DIM ANALOG</b>				
	MIS 5.DIM.330	MIS 5.DIM.374	MIS 5.DIM.500	★
<b>SLEEVE</b> for plaster model Stainless Steel				
	DIM 5.XSL.A10	DIM 5.XSL.A20	DIM 5.XSL.A30	★

# N-SERIES DIM ANALOG

compatible to: Straumann / SynOcta®

				
<b>PLATFORM</b>	3,5 mm NN	4,8 mm RN	6,5 mm WN	
<b>DIM ANALOG</b>				
	N 5.DIM.350	N 5.DIM.480	N 5.DIM.650	★
<b>SLEEVE</b> for plaster model Stainless Steel				
	DIM 5.XSL.A10	DIM 5.XSL.A20	DIM 5.XSL.A30	★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

NEW

# NEO-SERIES DIM ANALOG

compatible to: *NEOSS Implant System® / NEOSS™*



**PLATFORM**

3,5 - 5,5 mm

**DIM ANALOG**



NEO 5.DIM.355 ★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A20 ★

# R-SERIES DIM ANALOG

compatible to: *Zimmer Dental / Tapered Screw-Vent®*



**PLATFORM**

3,5 mm

4,5 mm

5,7 mm

**DIM ANALOG**



R 5.DIM.350

R 5.DIM.450

R 5.DIM.570 ★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A30 ★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA



# S-SERIES DIM ANALOG

compatible to: DENTSPLY Implants® / Astra Tech Implant System OsseoSpeed® TX



**PLATFORM**

3,5 / 4,0 mm

4,5 / 5,0 mm

**DIM ANALOG**



S 5.DIM.354

S 5.DIM.455

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

★

# SEV-SERIE DIM ANALOG

compatible to: DENTSPLY Implants® / Astra Tech Implant System™ EV

**NEW**



**PLATFORM**

3,0 mm

3,6 mm

4,2 mm

4,8 mm

5,4 mm

**DIM ANALOG**



SEV 5.DIM.300

SEV 5.DIM.360

SEV 5.DIM.420

SEV 5.DIM.480

SEV 5.DIM.540

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A30

DIM 5.XSL.A30

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# T-SERIES DIM ANALOG

compatible to: DENTSPLY Implants® / Xive®

				
<b>PLATFORM</b>	3,4 mm	3,8 mm	4,5 mm	5,5 mm
<b>DIM ANALOG</b>				
	T 5.DIM.340	T 5.DIM.380	T 5.DIM.450	T 5.DIM.550 ★
<b>SLEEVE</b> for plaster model Stainless Steel				
	DIM 5.XSL.A10	DIM 5.XSL.A20	DIM 5.XSL.A20	DIM 5.XSL.A30 ★

# THO-SERIES DIM ANALOG

compatible to: Thommen Medical® / SPI®



					
<b>PLATFORM</b>	3,5 mm	4,0 mm	4,5 mm	5,0 mm	6,0 mm
<b>DIM ANALOG</b>					
	THO 5.DIM.350	THO 5.DIM.400	THO 5.DIM.450	THO 5.DIM.500	THO 5.DIM.600 ★
<b>SLEEVE</b> for plaster model Stainless Steel					
	DIM 5.XSL.A10	DIM 5.XSL.A20	DIM 5.XSL.A20	DIM 5.XSL.A30	DIM 5.XSL.A30 ★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

NEW

# UPR-SERIES DIM ANALOG

compatible to: Sweden & Martina Implantology™ / Premium Kohno®



**PLATFORM**

3,3 mm

3,8 mm

4,25 mm

5,0 mm

**DIM ANALOG**



UPR 5.DIM.330

UPR 5.DIM.380

UPR 5.DIM.420

UPR 5.DIM.500

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A10

DIM 5.XSL.A20

DIM 5.XSL.A20

DIM 5.XSL.A30

★

# UTG-SERIES DIM ANALOG

compatible to: Sweden & Martina Implantology™ / Premium TG®



**PLATFORM**

3,3 - 4,25 mm

5,0 mm

**DIM ANALOG**



UTG 5.DIM.334

UTG 5.DIM.500

★

**SLEEVE**

for plaster model  
Stainless Steel



DIM 5.XSL.A20

DIM 5.XSL.A30

★

NEW

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 🇺🇸

# NOTES

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

---

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with \* are available in the USA 

# TABLE OF CONTENTS

NT CATALOGUE 2017-1

<b>1</b>	<b>TITANIUM BASE ABUTMENT</b>	10 – 49
<b>2</b>	<b>2-CONnect® ABUTMENT</b>	50 – 117
<b>3</b>	<b>NT-PREFORMS® ABUTMENT</b>	118 – 147
<b>4</b>	<b>DIM ANALOG</b>	148 – 161
<b>5</b>	<b>SURGICAL GUIDE SLEEVES</b>	163 – 165
<b>6</b>	<b>TOOLS &amp; DISCS</b>	167 – 181
<b>7</b>	<b>NT-iDent</b>	182 – 189
<b>8</b>	<b>SPECIFICATION</b>	190 – 191



# SURGICAL GUIDE SLEEVES

Step Drill Sleeves / Pilot Drill Sleeves



## FEATURES:

- Sleeve positioning by retentive fixture, no gluing necessary
- Easy and precise sleeve placement in the surgery guide by using the nt-insertion tool
- The optimized sleeve design also allows the use in narrow interdental spaces
- A drill mark on the sleeves upper edge facilitates the alignment when inserting into the surgery guide
- nt- trading drill sleeves are released in 3shape® Implant Studio for application




## APPLICATION:

- For preparing the implant bed by using implant surgical drills
- Compatible to the appropriate implant surgery sets



## TECHNICAL DETAILS:

- Titanium Grade 5 ELI



d = INNER DIAMETER | D = OUTER DIAMETER | DD = TREAD DIAMETER | L = LENGTH | SW = WIDTH












Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with \* are available in the USA

# SURGICAL GUIDE SLEEVES





Step Drill Sleeves / Pilot Drill Sleeves



## SURGICAL GUIDE SLEEVES

	ART. NO.	SYSTEM	d	D	DD	L	SW	
	SGS 16.SD4.148	NobelBiocare™ NP	Ø 4,10 mm	4,80 mm	5,80 mm	4,00 mm	4,50 mm	★
	SGS 16.SD5.060	NobelBiocare™ RP	Ø 5,00 mm	6,00 mm	7,00 mm	4,00 mm	5,70 mm	★
	SGS 16.SD6.270	NobelBiocare™ WP	Ø 6,20 mm	7,00 mm	8,00 mm	4,00 mm	6,70 mm	★
	SGS 16.SD3.548	Camlog®	Ø 3,50 mm	4,80 mm	5,80 mm	3,00 mm	4,50 mm	★
	SGS 16.SD4.563	Camlog®	Ø 4,50 mm	6,00 mm	7,00 mm	3,00 mm	5,70 mm	★
	SGS 16.SD4.560	Ankylos®/Xive® ND	Ø 4,48 mm	6,00 mm	7,00 mm	4,00 mm	5,70 mm	★
	SGS 16.SD4.960	Ankylos® WD	Ø 4,90 mm	6,00 mm	7,00 mm	4,00 mm	5,70 mm	★
	SGS 16.SD5.260	Xive® WD	Ø 5,20 mm	6,00 mm	7,00 mm	4,00 mm	5,70 mm	★
	SGS 16.SD5.060	Straumann	Ø 5,00 mm	6,00 mm	7,00 mm	4,00 mm	5,70 mm	★
	SGS 16.SD4.760	Astra	Ø 4,70 mm	6,00 mm	7,00 mm	4,00 mm	5,70 mm	★
	SGS 16.SD5.770	Astra	Ø 5,70 mm	7,00 mm	8,00 mm	4,00 mm	6,70 mm	★

## SINGLE SLEEVES

	ART. NO.	SYSTEM	d	D	DD	L	SW	
	SGS 16.PD2.032	Pilot drill-2,0 mm	2,00 mm	3,20 mm	4,20 mm	4,00 mm	2,90 mm	★
	SGS 16.PD2.232	Pilot drill-2,2 mm	2,20 mm	3,20 mm	4,20 mm	4,00 mm	2,90 mm	★
	SGS 16.PD2.332	Pilot drill-2,3 mm	2,35 mm	3,20 mm	4,20 mm	4,00 mm	2,90 mm	★
	SGS 16.PD2.848	Pilot drill-2,8 mm Straumann	2,80 mm	4,80 mm	5,80 mm	4,00 mm	4,50 mm	★

d = INNER DIAMETER | D = OUTER DIAMETER | DD = TREAD DIAMETER | L = LENGTH | SW = WIDTH

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 






# TABLE OF CONTENTS

NT CATALOGUE 2017-1

<b>1</b>	<b>TITANIUM BASE ABUTMENT</b>	<b>10 – 49</b>
<b>2</b>	<b>2-CONnect® ABUTMENT</b>	<b>50 – 117</b>
<b>3</b>	<b>NT-PREFORMS® ABUTMENT</b>	<b>118 – 147</b>
<b>4</b>	<b>DIM ANALOG</b>	<b>148 – 161</b>
<b>5</b>	<b>SURGICAL GUIDE SLEEVES</b>	<b>163 – 165</b>
<b>6</b>	<b>TOOLS &amp; DISCS</b>	<b>167 – 181</b>
<b>7</b>	<b>NT-iDent</b>	<b>182 – 189</b>
<b>8</b>	<b>SPECIFICATION</b>	<b>190 – 191</b>



# PROSTHETIC TOOLS



## TOOL SET

in wooden box contains W 11.000.000 Torque ratchet, W 11.100.000 Insert Holder, and the inserts W 11.MEX.G01, W 11.NEO.G02, W 11.SMU.G03, W 11.THO.G04, W 11.IRS.G10, W 11.THC.G20, W 11.Y00.G30, W 11.LN0.G40, W 11.EFK.G50, W 11.005.G60, W 11.VAL.G70

W 11.000.001

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# PROSTHETIC TOOLS

## TORQUE RATCHET

continuously adjustable to max. 40 Ncm  
ISO-Shaft connection



W 11.000.000



## INSERT-HOLDER

for changeable inserts (without ISO-Shaft)  
ISO-Shaft connection



W 11.100.000



## INSERT

for Insert-Holder and Torque Ratchet  
ISO-Shaft for MEX-Series  
(1,40 mm)



W 11.MEX.G01



## INSERT

for Insert-Holder and Torque Ratchet  
ISO-Shaft for NEO-Series



W 11.NEO.G02



## INSERT

for Insert-Holder and Torque Ratchet  
ISO-Shaft for SEV-, UPR- and UTG-Series  
(1,30 mm)



W 11.SMU.G03



## INSERT

for Insert-Holder and Torque Ratchet  
ISO-Shaft for THO-Series  
4-socket



W 11.THO.G04



## INSERT

for Insert-Holder and Torque Ratchet  
ISO-Shaft for BEG-, BIO-, I-, MIC-, MIS-,  
R- and S-Series  
(1,26 mm)






W 11.IRS.G10



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# PROSTHETIC TOOLS

<p><b>INSERT</b> for Insert-Holder and Torque Ratchet ISO-Shaft for T-, H-, CAM-, COL-, HIO-Series and DIM-Analog screw nut (1,20 mm)</p>	 	<p>W 11.THC.G20 ★</p>
<p><b>INSERT</b> for Insert-Holder and Torque Ratchet ISO-Shaft for Ankylos® (1,00 mm)</p>	 	<p>W 11.Y00.G30 ★</p>
<p><b>INSERT</b> for Insert-Holder and Torque Ratchet ISO-Shaft for BRE-, L- and N-Series, 2-CONnect® Coping screws Torx T6</p>	 	<p>W 11.LN0.G40 ★</p>
<p><b>INSERT</b> for Insert-Holder and Torque Ratchet ISO-Shaft for E-, F- and K-Series</p>	 	<p>W 11.EFK.G50 ★</p>
<p><b>INSERT</b> for Insert-Holder and Torque Ratchet ISO-Shaft for 2-CONnect®-Male Part, (2,10 mm)</p>	 	<p>W 11.005.G60 ★</p>
<p><b>INSERT</b> for Insert-Holder and Torque Ratchet ISO-Shaft for Validation Jig, (1,50 mm)</p>	 	<p>W 11.VAL.G70 ★</p>
<p><b>INSERT</b> for Insert-Holder and Torque Ratchet ISO- Shaft for Validation Jig, (1,50 mm) - ball head</p>	 	<p>W 11.VAL.G75 ★</p>

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# PROSTHETIC TOOLS

NEW



## SCREWDRIVER-SET

contains Screwdriver, details as on the following pages:

W 11.000.SET (6 / 11 pieces)

★

Notice: Products indicated with © and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# PROSTHETIC TOOLS

**SCREWDRIVER**

incl. ISO-Shaft for Torque Ratchet  
for 2-CONnect®-Male Part



W 11.2CO.NM0

★

**SCREWDRIVER**

incl. ISO-Shaft for Torque Ratchet  
for E-, F- and K-Series UG




W 11.EFK.000

★

**SCREWDRIVER**

incl. ISO-Shaft for Torque Ratchet  
for BEG-, BIO-, I-, MIC-, MIS-, R- and S-Series  
Hex 0,05“ (1,26 mm)



W 11.IRS.000

★

**SCREWDRIVER**

incl. ISO-Shaft for Torque Ratchet  
for BRE-, L- and N-Series, 2-CONnect®  
Coping screws Torx T6




W 11.LN2.COF

★

**SCREWDRIVER**

incl. ISO-Shaft for Torque Ratchet  
for MEX-Series



W 11.MEX.000

★

**SCREWDRIVER**

incl. ISO-Shaft for Torque Ratchet  
for NEO-Series



W 11.NEO.000

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA

# PROSTHETIC TOOLS

## SCREWDRIVER

incl. ISO-Shaft for Torque Ratchet  
for SEV-, UPR- and UTG-Series



W 11.SEV.SMU

★

## SCREWDRIVER

incl. ISO-Shaft for Torque Ratchet  
for T-, H-, CAM-, COL-, HIO-Series  
and DIM-Analog screw nut  
(1,20 mm)



W 11.THC.DIM

★

## SCREWDRIVER

incl. ISO-Shaft for Torque Ratchet  
for THO-Series, 4-socket



W 11.THO.000

★

## SCREWDRIVER

incl. ISO-Shaft for Torque Ratchet  
for coloured milling screw THO-Series  
4-socket



W 11.THO.MIL

★

## SCREWDRIVER

incl. ISO-Shaft for Torque Ratchet  
for Ankylos®  
(1,00 mm)




W 11.Y00.000


















★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# SURGICAL GUIDE SLEEVE TOOLS



## Surgical Guide Sleeves

	ART. NO.		SYSTEM	d	
	W 16.SGS.000	Handle	universal	—	★
	W 16.SGS.100	Blade	universal	—	★
	W 16.SGS5.120	SGS Positioning Tool	Pilot drill-2,0 mm	Ø 2,00 mm	★
	W 16.SGS5.122	SGS Positioning Tool	Pilot drill-2,2 mm	Ø 2,20 mm	★
	W 16.SGS5.123	SGS Positioning Tool	Pilot drill-2,3 mm	Ø 2,35 mm	★
	W 16.SGS5.228	SGS Positioning Tool	Pilot drill-2,8 mm Straumann	Ø 2,80 mm	★
	W 16.SGS5.235	SGS Positioning Tool	Camlog®	Ø 3,50 mm	★
	W 16.SGS5.241	SGS Positioning Tool	NobelBiocare™ NP	Ø 4,10 mm	★
	W 16.SGS5.345	SGS Positioning Tool	Ankylos®/Xive® ND	Ø 4,48 mm	★
	W 16.SGS5.345	SGS Positioning Tool	Camlog®	Ø 4,50 mm	★
	W 16.SGS5.347	SGS Positioning Tool	Astra	Ø 4,70 mm	★
	W 16.SGS5.349	SGS Positioning Tool	Ankylos® WD	Ø 4,90 mm	★
	W 16.SGS5.350	SGS Positioning Tool	NobelBiocare™ RP	Ø 5,00 mm	★
	W 16.SGS5.350	SGS Positioning Tool	Straumann	Ø 5,00 mm	★
	W 16.SGS5.352	SGS Positioning Tool	Xive® WD	Ø 5,20 mm	★
	W 16.SGS5.457	SGS Positioning Tool	Astra	Ø 5,70 mm	★
	W 16.SGS5.462	SGS Positioning Tool	NobelBiocare™ WP	Ø 6,20 mm	★

d = INNER DIAMETER

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 



# SINTER COMPONENTS

*Sinter pearls for dental CAD/CAM technology*

## SINTERIZATION OF ZR-OXIDE SUBSTRUCTURES



### ADVANTAGES:

Sinterization of Zr-oxide substructures. Full ceramics are the answer to patients demands for highly esthetic, metal-free and durable restorations. Zr-oxide became a common substructure for dental restorations already quite a while ago. This material features outstanding biocompatibility and mechanical properties. Zr-oxide is mechanically machined in its green stage, taking into consideration the specific shrinkage of this material. The sinterization is optimized for the specific material and is oversized milling relative to the material properties, thus assuring the best possible fit.

Another important factor contributing to a perfect fit is the right choice of support for this to be sintered substructure. Every manufacturer has his own recommendations concerning this supports. Some

suggest to sinter on special „pearls“, unfortunately particle size and quality are not always right to by example avoid getting pinched between the interproximals and thus distorting the bridge.

Other solutions favour the use of „drops“, resting on very expensive and fragile support discs. The necessary preparations for this type of support are always time consuming, sometimes even cumbersome and always generating additional costs. A viable alternative are special hi-density and quality sinterization pearls from nt-trading, optimized for crowns and bridges and therefore avoiding the common „pinching“ and distortion problems especially known to bridges.


**NT-PEARLS (200 G)**

W 14.182.000

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# DENTOKEEP PEEK DISC

*Dentokeep PEEK discs for milling fabrication of dentures in CAM process*



## **BENEFITS:**

- biocompatible
- MMA and benzoyl peroxide-free
- sterilizable
- high fracture strength
- low thermo conductivity
- low plaque affinity
- for composite veneering
- high abrasion resistance



## **APPLICATION:**

- monolithic crowns (alternative to metal anatomical crowns )
- implant fixed structures (bars, abutments, bridges combined with titanium bases) - dental telescopes, bar riders
- individual gingiva forming
- tabletops
- temporary prosthetics
- crowns / bridges ( for composite veneering )
- occlusal splints



## **TECHNICAL DETAILS:**

- tensile modulus of elasticity:  $\geq 3800$  MPa
- density: 1,30 – 1,50 g/cm<sup>3</sup>
- color: pearl white, A, GUM
- melting temperature: 343 °C
- 14 mm, 18 mm, 23 mm thickness
- diameter 98,5 mm

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# DENTOKEEP PEEK DISC

*Dentokeep PEEK discs for milling fabrication of dentures in CAM process*




## DENTOKEEP

nt-trading Dentokeep PEEK Disc are blanks for technical milling manufacture of permanent dentures and prosthetic brace in the CAM process. The derived prosthetic designs are available on the remaining teeth, can be attached to stumps and / or implant abutment provide a basic functional and aesthetic care.

1. PEEK Disc 98.5 mm, pearl white, A, GUM,14 mm, 18 mm and 23 mm thick
2. For CAD/CAM Technology
3. Clip in prosthetics CAD/CAM
4. Class II product for permanent prosthetic restorations




### DENTOKEEP

PEEK Disc  
Size 14 mm

			
Art. No.	12.000.P14	12.00A.P14	12.GUM.P14
Color	Pearl white	A	GUM




### DENTOKEEP

PEEK Disc  
Size 18 mm

			
Art. No.	12.000.P18	12.00A.P18	12.GUM.P18
Color	Pearl white	A	GUM

### DENTOKEEP

PEEK Disc  
Size 23 mm

			
Art. No.	12.000.P23	12.00A.P23	12.GUM.P23
Color	Pearl white	A	GUM

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# DENTOMODEL DISC

*Dentomodel discs for milling fabrication of dental master models in cam proces*



## **BENEFITS:**

- high edge stability
- abrasion-stable
- high design accuracy
- aging resistant



## **APPLICATION:**

- for milling manufacture of dental master models and saw cut models



## **TECHNICAL DETAILS:**

- color: ivory
- diameter 98,5 mm
- 25 mm, 28 mm, 30 mm thickness

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with \* are available in the USA 

# DENTOMODEL DISC

*Dentomodel discs for milling fabrication of dental master models in cam process*

## DENTOMODEL

nt-trading DENTOMODEL blanks are developed especially for the technical milling manufacture of physical dental models based on intra-oral scan data. It provides a high edge stability and design accuracy for dental master models. It's very abrasion-stable and has no significant dimension change by aging compared to plaster models.

1. Model Disc 98,5 mm, ivory, 25 mm, 28 mm and 30 mm thick
2. Color: Ivory
3. For CAD/CAM Technology Model

### DENTOMODEL

MODEL Disc  
Size 25 mm



21.000.M25

### DENTOMODEL

MODEL Disc  
Size 28 mm



21.000.M28

### DENTOMODEL

MODEL Disc  
Size 30 mm



21.000.M30

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with \* are available in the USA 

# SCAN EQUIPMENT

## NT-OptiScan™ Spray



### ADVANTAGES:

- Optimize composition
- Perfect dosage with proven applicator
- Optimize preparation of your working model for optical scanning with modern dental scanner
- Economical application
- Water soluble
- Handy size: Volume 75 ml brutto
- Superior scanning results
- Special attractive price

NT-OPTISCAN™ SPRAY

W 14.61101

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with \* are available in the USA 

# NT-MILLING AND GRINDING TOOLS

nt-trading tools are specially developed for dental CAD/CAM systems with a 3 mm piston. They are up to the high mark to process dental materials and are constant liable to quality checks. Tools coated with tax are especially qualified for process of dental high-capacity plastics, as well as for process of milling wax. Tools coated with diamonds are especially qualified for process of abrasive materials like zirconium dioxide.

## CLAMPING SLEEVE

adaption for grinding shaft from Ø 3,0 mm to Ø 6,0 mm.



11000

—

—

★

## NT-DIABURR

The milling tool coated with diamonds nt-Diaburr offers you a lifetime of at least 350 units while process of ZrO<sub>2</sub> with the milling machine.



Ø 0,6 mm



Ø 1,0 mm



2,5 mm

11100

11101

11102

★

## NT-UBURR

Universal milling tools are qualified for process of plastics, waxes and ZrO<sub>2</sub> with the milling machine. Depending on choice of material. Nt-Uburr offers you a lifetime of at least 175 units.



Ø 1,0 mm



Ø 2,5 mm

11201

11202

—

★

## NT-PEEKBURR

Special milling tools are qualified for process of PEEK materials like DENTOKEEP, and plastics.



Ø 1,0 mm



Ø 2,5 mm

11301

11302

—

★

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 

# NT-IQ LIBRARY

Free digital implant library for CAD process




## BENEFITS:

The nt-IQ implant library enables you to design individual prosthetic solutions for almost all current implant systems. You are able to fabricate individual milled structures in your own lab, for glued or one-piece structures with a maximum of precision and individuality.



### nt-IQ Library contains:

- titanium bases
- 2-CONnect® system
- nt-Preforms® (one-piece abutments)
- DIM analogs



## APPLICATION:

- individual ceramic abutments on titanium bases
- individual one-piece titanium abutments
- occlusal screwable crowns and bridges
- bars, telescopes
- digital implant model manufacturing by DIM analogs



Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with ★ are available in the USA 



# TABLE OF CONTENTS

NT CATALOGUE 2017-1

<b>1</b>	<b>TITANIUM BASE ABUTMENT</b>	10 – 49
<b>2</b>	<b>2-CONnect® ABUTMENT</b>	50 – 117
<b>3</b>	<b>NT-PREFORMS® ABUTMENT</b>	118 – 147
<b>4</b>	<b>DIM ANALOG</b>	148 – 161
<b>5</b>	<b>SURGICAL GUIDE SLEEVES</b>	163 – 165
<b>6</b>	<b>TOOLS &amp; DISCS</b>	167 – 181
<b>7</b>	<b>NT-iDent</b>	182 – 189
<b>8</b>	<b>SPECIFICATION</b>	190 – 191




# TECHNOLOGY CENTER

## SERVICES AT A GLANCE

The NTiDent technology center gives you the opportunity to offer high-precision and certified implant supra structures in addition to your current manufacturing capacity and product portfolio.



- Production of digital implant models in combination with the production of crowns, bridges/bars and custom abutments
- Custom made abutments
- Manufacture of directly screw retained bridges/bars on implants as well as meso/tertiary structures in materials as CoCr, Peek (Dentokeep), and titanium
- Crowns and bridges in materials as Zirconium, E.max® CAD, PMMA, Peek (Dentokeep), CoCr and titanium
- Safety tested through highest production and quality standards
- Scan and design service



# SERVICE PORTFOLIO



**COCR / TITANIUM**



**CUSTOM ABUTMENTS / ATTACHMENTS**




**ZIRCONIUM / PEEK / PMMA**





- Implant analog for digital model manufacture
- Two-piece implant analog
- Exactly positionable
- Position correction possible




# PROCESS OPERATIONS




## CUSTOM ABUTMENTS



## DIGITAL IMPLANT MODEL MANUFACTURE AND PRODUCTION OF BRIDGES/BARS/CUSTOM ABUTMENTS



## BRIDGES/BARS/CUSTOM ABUTMENTS

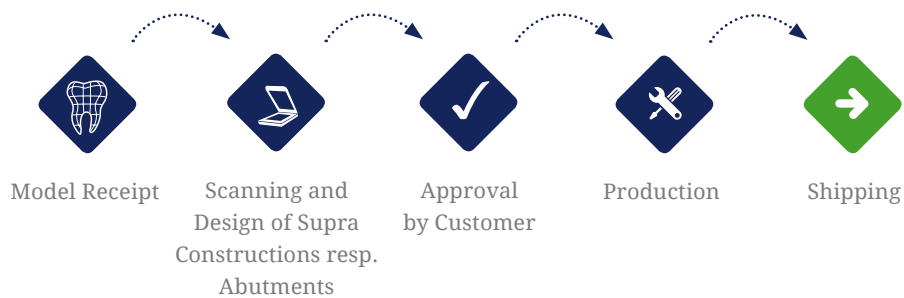

# SENDING DATA AND SHIPPING OF MODELS



## DATATRANSFER

- FTP-Server
- E-mail: [nt-iDent@nt-trading.com](mailto:nt-iDent@nt-trading.com)  
(up to a maximum of 5 MB)



## MODELTRANSFER


- Please send it to the following address:  
**nt-trading GmbH & Co. KG**  
**G.-Braun-Str. 18**  
**76187 Karlsruhe**  
**Germany**



## NTiDent DELIVERY TIMES

- Individually manufactured abutments: **1-2 workdays** after data receipt, **2-3 workdays** after model receipt
- bridges/bars: **3 workdays** after data receipt, **5 workdays** after model receipt

# PROVED DIGITAL IMPLANT WORKFLOW

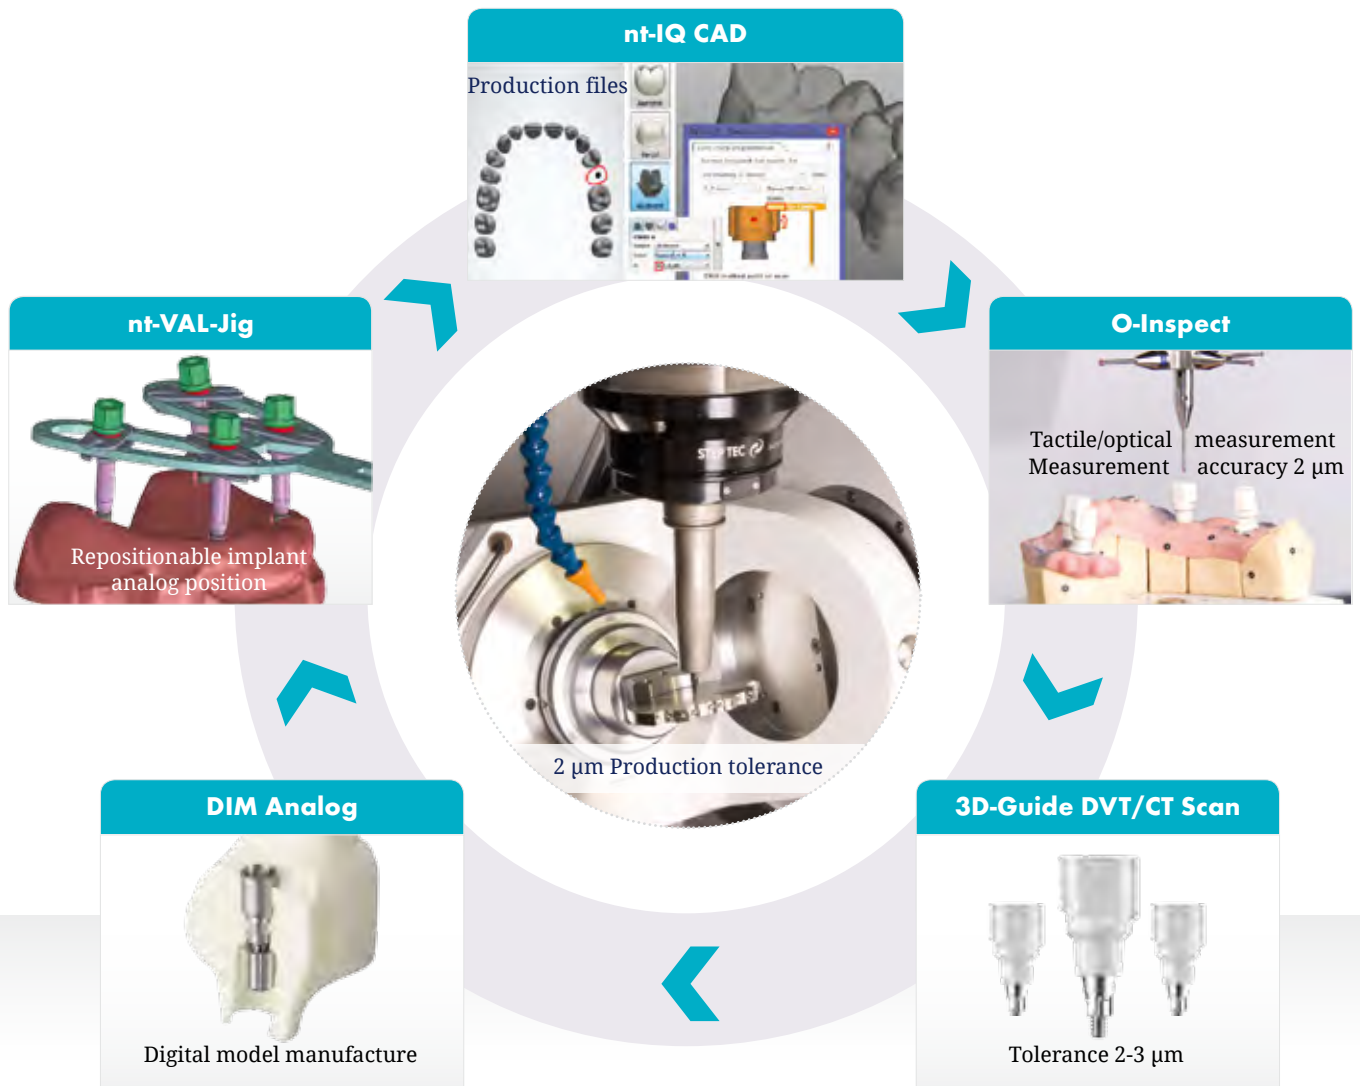

**nt-trading GmbH & Co. KG**

G.-Braun-Str.18

76187 Karlsruhe/Germany



Phone: +49 (0)721 / 91 54 71 60

Fax: +49 (0)721 / 91 54 71 61



info@nt-trading.com

www.nt-iDent.com

**NT***iDent*

# TIGHTENING TOURQUES

## Titanium Base / Abutments / nt-Preform®

NCM	ABUTMENT
15 Ncm	THO-Series 3,5
20 Ncm	CAM-Series / COL-Series / H-Series / HIO-Series 3,5
25 Ncm	BRE-Series / F-Series 3,5 / S-Series / SEV-Series / T-Series / THO-Series 4,0 - 6,0 / UPR-Series / UTG-Series
30 Ncm	BEG-Series / BIO-Series / HIO-Series 4,0 - 6,0 / MEX-Series / MIC-Series / MIS-Series / NEO-Series / R-Series
35 Ncm	E-Series / F-Series 4,3 - 5,0 / I-Series / K-Series / L-Series / N-Series

## 2-CONnect®

NCM	STRAIGHT ABUTMENT	COPING WITH SCREW KS 61	COPING WITH SCREW KS 60
15 Ncm	THO-Series 3,5	CAM-Series 3,3 / COL-Series 3,3 / HIO-Series 3,5	H-Series / R-Series / T-Series 3,4 / THO-Series 3,5 - 4,0
20 Ncm	CAM-Series 3,3 / COL-Series 3,3 / H-Series / HIO-Series 3,5	BRE-Series / F-Series 3,5 / S-Series / SEV-Series / T-Series 3,8 - 4,5 / THO-Series 4,0 - 6,0 / UPR-Series / UTG-Series	—
25 Ncm	BRE-Series / F-Series 3,5 / S-Series / SEV-Series / T-Series / THO-Series 4,0 - 6,0 / UPR-Series / UTG-Series	BEG-Series / BIO-Series / CAM-Series 3,8 - 5,0 / COL-Series 3,8 - 5,0 / HIO-Series 4,0 - 6,0 / MEX-Series / MIC-Series / MIS-Series / NEO-Series	—
30 Ncm	BEG-Series / BIO-Series / CAM 3,8 - 5,0 / HIO-Series 4,0 - 6,0 / MEX-Series / MIC-Series / MIS-Series / NEO-Series / R-Series / COL-Series 3,8 - 5,0	E-Series / F-Series 4,3 - 5,0 / L-Series / N-Series	—
35 Ncm	E-Series / F-Series 4,3 - 5,0 / L-Series / N-Series	—	—

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures. Products indicated with \* are available in the USA 



# TIGHTENING TORQUES

## 2-CONnect® ANGLED ABUTMENT

NCM	M-ABUTMENT	COPING WITH SCREW KS 62
15 Ncm	—	All Implant Series
20 Ncm	All Implant Series	—



### ADDITIONAL INFORMATION TO OUR PRODUCTS SUCH AS:

Instruction For Use, Videos, News and product updates, Useful information can be found on [www.nt-trading.com](http://www.nt-trading.com)

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

# COLOURED MILLING SCREW



The delivered, coloured marked screw, will be used as Milling or Lab Screw for the nt-Preform® Abutment. For all Implant Series and diameters you have to use a Screwdriver with Torx T6. Exception is THO-Series (Thommen Medical), with a 4-lobe screwdriver.

For the fixing of the Milling Screw (10 Ncm) on un-machined nt-Preform® Abutment, you have to use the long-shaft screwdriver with article-number W 12.WS0.000 and for Thommen W 11.TH0.MIL.

For the fixing of the Milling Screw on finished milled nt-Preform Abutment, can be used from the column Lab-screw.

## USAGE COLOURED MILLING SCREW

SERIES	LAB	MILLING	TORQUE
All Implant Series (except THO-Series)	W 11.LN0.G40 on page 170	W 12.WS0.000 on page 144	10 Ncm
	W 11.LN2.COF on page 172		10 Ncm
THO-Series	W 11.TH0.G04 on page 169	W 11.TH0.MIL on page 144	10 Ncm
	W 11.TH0.000 on page 173		10 Ncm

Notice: Products indicated with ® and ™ are registered brand names of the respective manufactures.  
Products indicated with ★ are available in the USA 

The logo consists of the letters 'NT' in a bold, blue, sans-serif font. The background of the entire page features a large, abstract graphic of overlapping triangles in shades of green and blue, creating a dynamic, geometric pattern.

*digital implant technology*

**NT**

nt-trading GmbH & Co. KG

G.-Braun-Straße 18

76187 Karlsruhe

Phone: +49 (0)721 / 915471-60

Fax: +49 (0)721 / 915471-61

Email: [info@nt-trading.com](mailto:info@nt-trading.com)

[www.nt-trading.com](http://www.nt-trading.com)